

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027995.D
 Acq On : 21 Sep 2022 05:08
 Operator : SY/MD
 Sample : N4674-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	103	rVB	215585	228138	15.42%	2.099%
2	1.561	155	162	179	rVB	177439	203339	13.75%	1.871%
3	2.102	320	330	350	rBV	360348	533308	36.05%	4.907%
4	2.503	447	455	458	rBV5	1337	2096	0.14%	0.019%
5	2.606	484	487	489	rBV	590	381	0.03%	0.004%
6	2.622	489	492	494	rBV2	558	372	0.03%	0.003%
7	2.706	517	518	521	rBV2	618	338	0.02%	0.003%
8	2.809	549	550	552	rBV2	841	264	0.02%	0.002%
9	2.905	578	580	581	rBV	848	271	0.02%	0.002%
10	2.950	592	594	597	rVB3	674	278	0.02%	0.003%
11	3.044	620	623	628	rBV4	517	516	0.03%	0.005%
12	3.092	635	638	640	rVB2	982	559	0.04%	0.005%
13	3.108	641	643	645	rVB3	827	296	0.02%	0.003%
14	3.159	656	659	661	rBV3	473	312	0.02%	0.003%
15	3.275	692	695	697	rBV3	628	344	0.02%	0.003%
16	3.310	702	706	707	rBV3	343	264	0.02%	0.002%
17	3.339	714	715	719	rBV3	656	459	0.03%	0.004%
18	3.388	727	730	734	rVB4	602	498	0.03%	0.005%
19	3.410	734	737	740	rBV3	530	292	0.02%	0.003%
20	3.487	759	761	765	rVB3	610	383	0.03%	0.004%
21	3.516	767	770	774	rBV3	678	563	0.04%	0.005%
22	3.548	778	780	781	rBV2	505	221	0.01%	0.002%
23	3.609	796	799	802	rBV3	545	444	0.03%	0.004%
24	3.664	813	816	817	rVB2	461	211	0.01%	0.002%
25	3.677	817	820	821	rBV2	1038	608	0.04%	0.006%
26	3.732	833	837	840	rBV3	662	517	0.03%	0.005%
27	3.809	859	861	865	rVB3	661	465	0.03%	0.004%
28	3.835	868	869	871	rBV	496	211	0.01%	0.002%
29	3.876	873	882	916	rBV	125185	370337	25.03%	3.408%
30	4.339	1011	1026	1056	rBV	242265	600715	40.61%	5.527%
31	4.648	1120	1122	1124	rBV	607	342	0.02%	0.003%
32	4.790	1164	1166	1168	rBV2	398	209	0.01%	0.002%
33	4.818	1171	1175	1177	rBV3	837	675	0.05%	0.006%
34	4.896	1193	1199	1200	rBV2	632	462	0.03%	0.004%
35	5.037	1227	1243	1268	rBV2	573767	1479342	100.00%	13.612%
36	5.465	1370	1376	1378	rBV5	821	833	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027995.D
 Acq On : 21 Sep 2022 05:08
 Operator : SY/MD
 Sample : N4674-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.497	1384	1386	1388	rBV3	813	398	0.03%	0.004%
38	5.609	1410	1421	1449	rBV	408102	837902	56.64%	7.710%
39	5.986	1536	1538	1540	rVB2	730	247	0.02%	0.002%
40	6.063	1549	1562	1582	rBV	335716	678542	45.87%	6.243%
41	6.346	1646	1650	1654	rVB4	1051	803	0.05%	0.007%
42	6.490	1693	1695	1699	rBV3	429	272	0.02%	0.003%
43	6.510	1699	1701	1705	rVV4	1031	541	0.04%	0.005%
44	6.535	1705	1709	1713	rBV5	1108	942	0.06%	0.009%
45	6.587	1723	1725	1728	rVB2	1224	551	0.04%	0.005%
46	6.603	1728	1730	1733	rBV3	749	458	0.03%	0.004%
47	6.619	1733	1735	1739	rVB3	852	689	0.05%	0.006%
48	6.815	1793	1796	1799	rBV4	614	400	0.03%	0.004%
49	6.831	1799	1801	1804	rBV2	577	321	0.02%	0.003%
50	6.921	1827	1829	1830	rBV	534	206	0.01%	0.002%
51	6.982	1837	1848	1875	rBV	161572	304641	20.59%	2.803%
52	7.310	1938	1950	1972	rBV	625374	1097434	74.18%	10.098%
53	7.584	2032	2035	2037	rBV2	954	648	0.04%	0.006%
54	7.619	2037	2046	2068	rVV2	112403	200098	13.53%	1.841%
55	7.838	2110	2114	2115	rBV3	677	421	0.03%	0.004%
56	7.998	2160	2164	2168	rBV5	821	701	0.05%	0.006%
57	8.021	2168	2171	2174	rBV4	566	404	0.03%	0.004%
58	8.085	2181	2191	2219	rBV	419696	763754	51.63%	7.027%
59	8.416	2292	2294	2298	rVB3	798	500	0.03%	0.005%
60	8.606	2351	2353	2356	rVB2	459	249	0.02%	0.002%
61	8.625	2356	2359	2361	rBV2	451	318	0.02%	0.003%
62	8.651	2365	2367	2369	rBV2	599	320	0.02%	0.003%
63	8.712	2382	2386	2387	rVB2	425	215	0.01%	0.002%
64	8.751	2396	2398	2401	rBV2	450	295	0.02%	0.003%
65	8.847	2417	2428	2453	rBV	588813	955032	64.56%	8.787%
66	9.162	2524	2526	2532	rVB4	1084	680	0.05%	0.006%
67	9.198	2535	2537	2542	rBV3	441	309	0.02%	0.003%
68	9.252	2546	2554	2559	rBV2	583	859	0.06%	0.008%
69	9.291	2562	2566	2567	rBV2	402	196	0.01%	0.002%
70	9.391	2594	2597	2600	rVB	421	254	0.02%	0.002%
71	9.410	2600	2603	2605	rBV	408	265	0.02%	0.002%
72	9.465	2618	2620	2625	rVB4	539	387	0.03%	0.004%
73	9.510	2631	2634	2640	rVB2	425	266	0.02%	0.002%
74	9.532	2640	2641	2645	rBV	324	244	0.02%	0.002%
75	9.567	2647	2652	2655	rVV4	377	405	0.03%	0.004%
76	9.600	2659	2662	2664	rBV2	538	321	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027995.D
 Acq On : 21 Sep 2022 05:08
 Operator : SY/MD
 Sample : N4674-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.612	2664	2666	2669	rVV2	537	222	0.02%	0.002%
78	9.680	2683	2687	2691	rBV3	635	422	0.03%	0.004%
79	9.776	2715	2717	2720	rVB3	808	311	0.02%	0.003%
80	10.014	2789	2791	2792	rBV	675	302	0.02%	0.003%
81	10.214	2841	2853	2875	rBV	484327	755717	51.08%	6.953%
82	10.426	2917	2919	2923	rBV5	864	526	0.04%	0.005%
83	10.503	2941	2943	2946	rBV3	1083	478	0.03%	0.004%
84	10.542	2953	2955	2957	rBV2	877	498	0.03%	0.005%
85	10.702	3003	3005	3006	rBV	645	318	0.02%	0.003%
86	10.899	3064	3066	3067	rBV2	700	312	0.02%	0.003%
87	11.124	3133	3136	3137	rBV2	708	404	0.03%	0.004%
88	11.185	3153	3155	3159	rBV2	711	455	0.03%	0.004%
89	11.246	3162	3174	3200	rBV	569113	872389	58.97%	8.027%
90	11.622	3279	3291	3312	rBV	602723	951465	64.32%	8.755%
91	12.034	3417	3419	3423	rVB4	1029	510	0.03%	0.005%
92	12.108	3440	3442	3444	rBV3	657	216	0.01%	0.002%
93	12.217	3474	3476	3480	rBV3	794	556	0.04%	0.005%
94	12.362	3518	3521	3522	rBV2	668	309	0.02%	0.003%
95	12.789	3652	3654	3656	rBV	519	267	0.02%	0.002%
96	12.892	3684	3686	3688	rBV3	582	344	0.02%	0.003%
97	13.062	3736	3739	3741	rBV3	843	449	0.03%	0.004%
98	13.619	3910	3912	3915	rBV2	783	374	0.03%	0.003%
99	13.696	3933	3936	3937	rBV	1080	602	0.04%	0.006%
100	13.741	3948	3950	3952	rBV	738	391	0.03%	0.004%




Sum of corrected areas: 10868188

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027995.D
Acq On : 21 Sep 2022 05:08
Operator : SY/MD
Sample : N4674-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

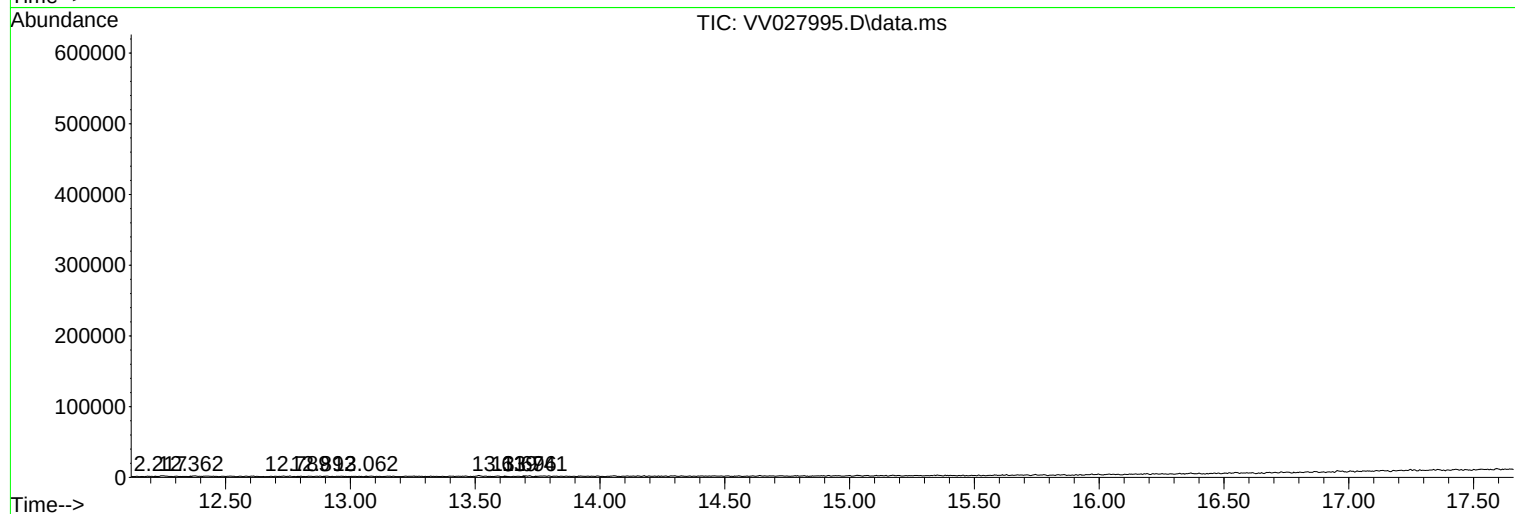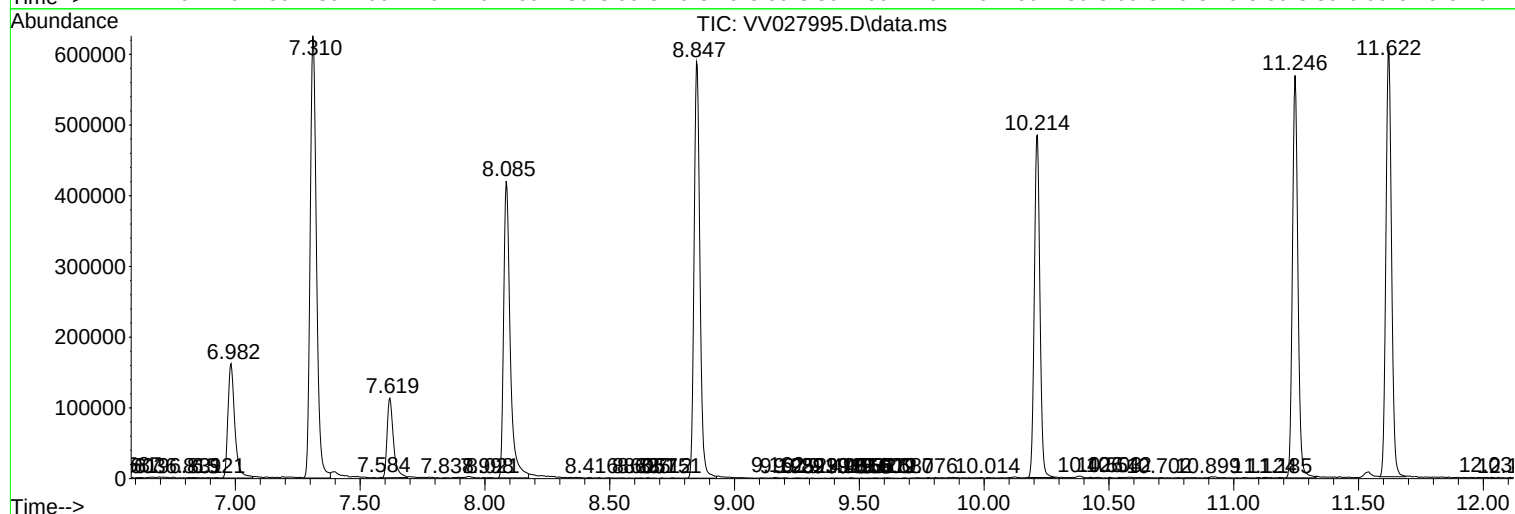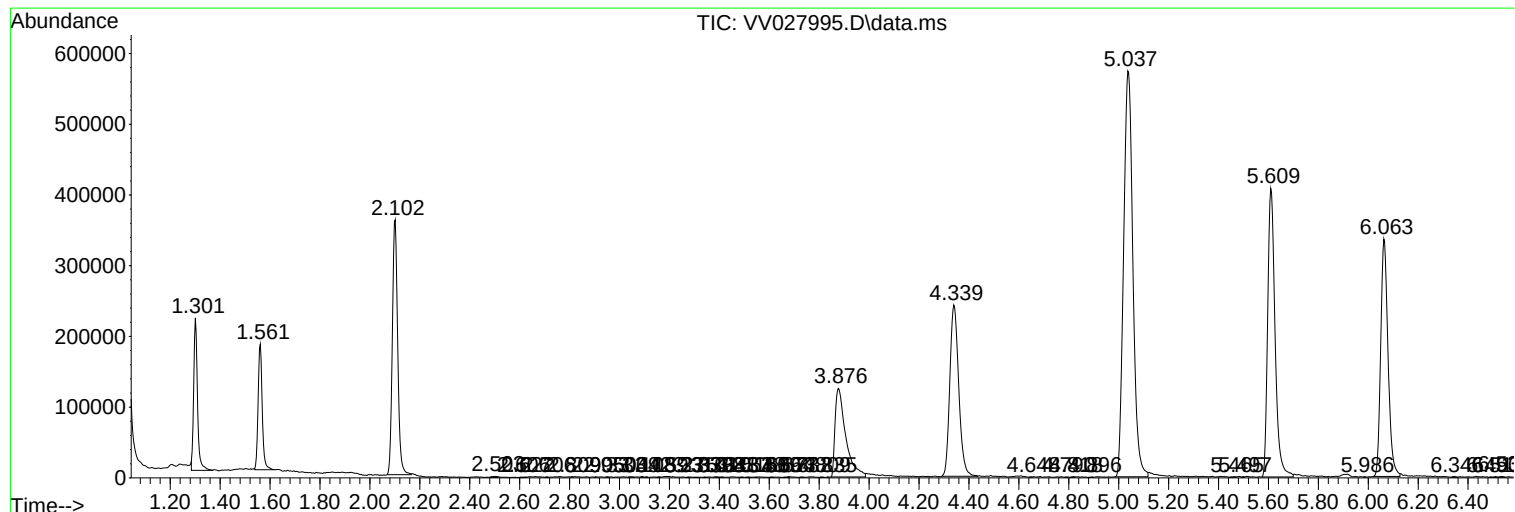

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027995.D
Acq On : 21 Sep 2022 05:08
Operator : SY/MD
Sample : N4674-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027995.D
Acq On : 21 Sep 2022 05:08
Operator : SY/MD
Sample : N4674-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc