

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027996.D
 Acq On : 21 Sep 2022 05:32
 Operator : SY/MD
 Sample : N4674-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	210205	222648	16.39%	2.022%
2	1.561	156	162	172	rVB	170527	183599	13.51%	1.667%
3	2.101	320	330	349	rVB2	379963	567665	41.79%	5.155%
4	2.288	383	388	390	rBV3	808	651	0.05%	0.006%
5	2.445	435	437	441	rBV4	468	299	0.02%	0.003%
6	2.587	478	481	484	rBV3	340	240	0.02%	0.002%
7	2.638	494	497	501	rBV	285	244	0.02%	0.002%
8	2.664	501	505	508	rBV2	619	621	0.05%	0.006%
9	2.719	520	522	526	rVB	362	257	0.02%	0.002%
10	2.754	528	533	537	rBV5	1011	1030	0.08%	0.009%
11	2.931	585	588	592	rVB3	316	253	0.02%	0.002%
12	2.957	593	596	598	rBV2	488	291	0.02%	0.003%
13	3.014	611	614	617	rVB2	591	330	0.02%	0.003%
14	3.182	661	666	670	rBV3	736	782	0.06%	0.007%
15	3.249	682	687	688	rBV2	472	291	0.02%	0.003%
16	3.288	696	699	704	rVB2	254	263	0.02%	0.002%
17	3.359	717	721	723	rBV3	371	259	0.02%	0.002%
18	3.410	735	737	742	rVV	456	307	0.02%	0.003%
19	3.494	760	763	767	rBV	446	343	0.03%	0.003%
20	3.648	806	811	813	rBV	323	291	0.02%	0.003%
21	3.876	873	882	916	rBV	114140	361820	26.63%	3.286%
22	4.259	999	1001	1004	rBV2	474	292	0.02%	0.003%
23	4.339	1010	1026	1048	rBV	222798	550752	40.54%	5.002%
24	4.606	1095	1109	1125	rBV3	5726	14805	1.09%	0.134%
25	4.664	1125	1127	1132	rVV4	677	584	0.04%	0.005%
26	4.889	1194	1197	1199	rBV2	426	259	0.02%	0.002%
27	4.931	1207	1210	1215	rBV3	363	376	0.03%	0.003%
28	5.040	1226	1244	1272	rBV2	527315	1358537	100.00%	12.338%
29	5.397	1353	1355	1358	rVV3	451	244	0.02%	0.002%
30	5.452	1368	1372	1374	rVB2	415	262	0.02%	0.002%
31	5.481	1378	1381	1383	rBV2	445	278	0.02%	0.003%
32	5.609	1409	1421	1452	rBV	383965	778420	57.30%	7.070%
33	5.908	1500	1514	1548	rBV	393178	784441	57.74%	7.124%
34	6.063	1550	1562	1591	rVV	297653	610476	44.94%	5.544%
35	6.336	1642	1647	1651	rBV2	836	753	0.06%	0.007%
36	6.368	1654	1657	1661	rVV3	718	405	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027996.D
 Acq On : 21 Sep 2022 05:32
 Operator : SY/MD
 Sample : N4674-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.397	1664	1666	1671	rVB3	611	420	0.03%	0.004%
38	6.426	1671	1675	1677	rBV2	457	297	0.02%	0.003%
39	6.464	1684	1687	1689	rVB3	496	238	0.02%	0.002%
40	6.516	1698	1703	1705	rBV3	454	247	0.02%	0.002%
41	6.526	1705	1706	1711	rVB3	532	340	0.03%	0.003%
42	6.551	1711	1714	1717	rBV2	563	405	0.03%	0.004%
43	6.712	1758	1764	1768	rBV5	773	907	0.07%	0.008%
44	6.809	1791	1794	1796	rBV2	546	351	0.03%	0.003%
45	6.982	1836	1848	1874	rBV2	150176	278833	20.52%	2.532%
46	7.162	1902	1904	1906	rBV2	439	276	0.02%	0.003%
47	7.310	1939	1950	1968	rBV	581277	1003420	73.86%	9.113%
48	7.619	2036	2046	2068	rBV	109741	189898	13.98%	1.725%
49	7.844	2110	2116	2119	rBV6	679	724	0.05%	0.007%
50	7.940	2139	2146	2154	rVB6	2469	3987	0.29%	0.036%
51	7.985	2158	2160	2164	rVB2	545	292	0.02%	0.003%
52	8.085	2180	2191	2216	rBV	390956	715819	52.69%	6.501%
53	8.448	2302	2304	2307	rBV3	666	497	0.04%	0.005%
54	8.580	2342	2345	2348	rBV	504	346	0.03%	0.003%
55	8.661	2366	2370	2371	rBV3	410	254	0.02%	0.002%
56	8.680	2371	2376	2379	rVV5	822	736	0.05%	0.007%
57	8.699	2380	2382	2387	rVB3	779	367	0.03%	0.003%
58	8.741	2393	2395	2400	rVB	399	257	0.02%	0.002%
59	8.847	2417	2428	2449	rBV	562973	925745	68.14%	8.408%
60	9.339	2579	2581	2588	rBV3	474	474	0.03%	0.004%
61	9.397	2596	2599	2600	rBV	434	251	0.02%	0.002%
62	9.596	2656	2661	2665	rBV6	751	825	0.06%	0.007%
63	9.641	2672	2675	2678	rVB2	460	316	0.02%	0.003%
64	9.976	2775	2779	2781	rBV	441	257	0.02%	0.002%
65	10.111	2819	2821	2822	rBV2	754	339	0.02%	0.003%
66	10.214	2835	2853	2872	rBV	439150	691952	50.93%	6.284%
67	10.381	2900	2905	2916	rVB5	2087	3208	0.24%	0.029%
68	10.580	2963	2967	2970	rVB3	1004	796	0.06%	0.007%
69	10.641	2982	2986	2990	rBV3	629	342	0.03%	0.003%
70	10.734	3013	3015	3021	rVB2	399	351	0.03%	0.003%
71	10.763	3021	3024	3026	rBV2	408	271	0.02%	0.002%
72	10.857	3049	3053	3058	rBV2	906	694	0.05%	0.006%
73	10.956	3079	3084	3085	rBV2	286	247	0.02%	0.002%
74	10.966	3085	3087	3092	rVV3	553	383	0.03%	0.003%
75	11.005	3095	3099	3104	rBV2	535	440	0.03%	0.004%
76	11.030	3104	3107	3109	rVB3	614	327	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027996.D
 Acq On : 21 Sep 2022 05:32
 Operator : SY/MD
 Sample : N4674-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.082	3119	3123	3125	rVB2	506	354	0.03%	0.003%
78	11.107	3125	3131	3132	rBV2	345	251	0.02%	0.002%
79	11.143	3139	3142	3143	rBV2	538	251	0.02%	0.002%
80	11.246	3162	3174	3192	rBV	540308	822869	60.57%	7.473%
81	11.541	3257	3266	3274	rBV5	3241	6476	0.48%	0.059%
82	11.622	3279	3291	3311	rBV	570547	903751	66.52%	8.208%
83	11.889	3372	3374	3378	rBV3	754	348	0.03%	0.003%
84	11.940	3387	3390	3392	rBV2	464	266	0.02%	0.002%
85	11.966	3396	3398	3400	rBV	480	263	0.02%	0.002%
86	12.249	3482	3486	3489	rBV3	617	626	0.05%	0.006%
87	12.320	3506	3508	3513	rVB3	521	321	0.02%	0.003%
88	12.349	3513	3517	3519	rBV2	509	380	0.03%	0.003%
89	12.464	3550	3553	3556	rBV3	460	410	0.03%	0.004%
90	12.496	3559	3563	3565	rBV2	336	248	0.02%	0.002%
91	12.789	3652	3654	3656	rBV2	554	312	0.02%	0.003%
92	12.802	3656	3658	3662	rVV3	416	335	0.02%	0.003%
93	12.873	3677	3680	3682	rBV2	726	459	0.03%	0.004%
94	12.979	3711	3713	3720	rVB4	974	882	0.06%	0.008%
95	13.246	3793	3796	3798	rBV2	731	505	0.04%	0.005%
96	13.480	3867	3869	3871	rBV	801	384	0.03%	0.003%
97	13.840	3979	3981	3984	rVB3	783	290	0.02%	0.003%
98	13.988	4025	4027	4030	rBV2	649	488	0.04%	0.004%
99	14.249	4104	4108	4110	rBV3	742	430	0.03%	0.004%
100	14.564	4202	4206	4209	rBV4	616	511	0.04%	0.005%




Sum of corrected areas: 11010907

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027996.D
Acq On : 21 Sep 2022 05:32
Operator : SY/MD
Sample : N4674-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

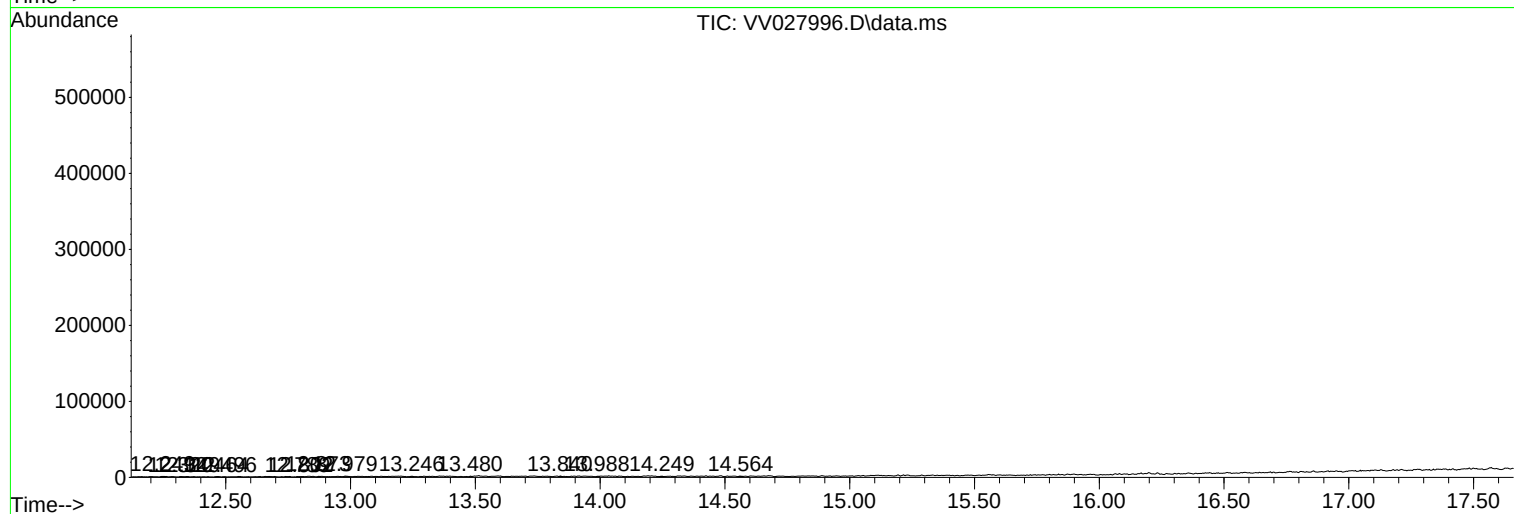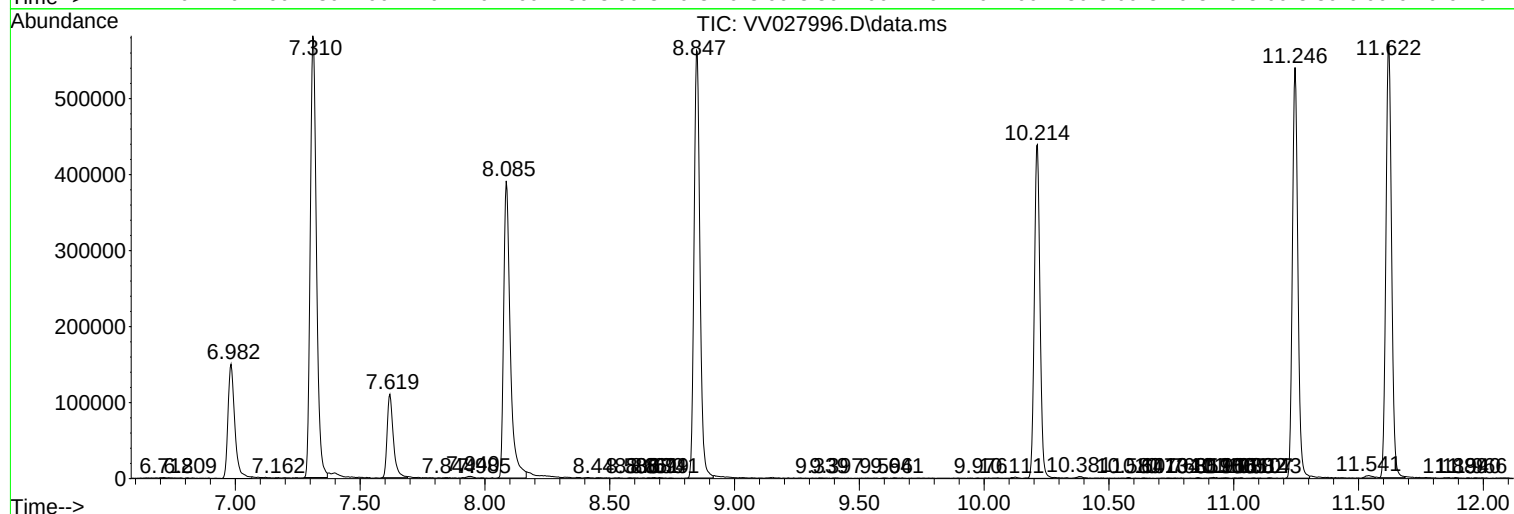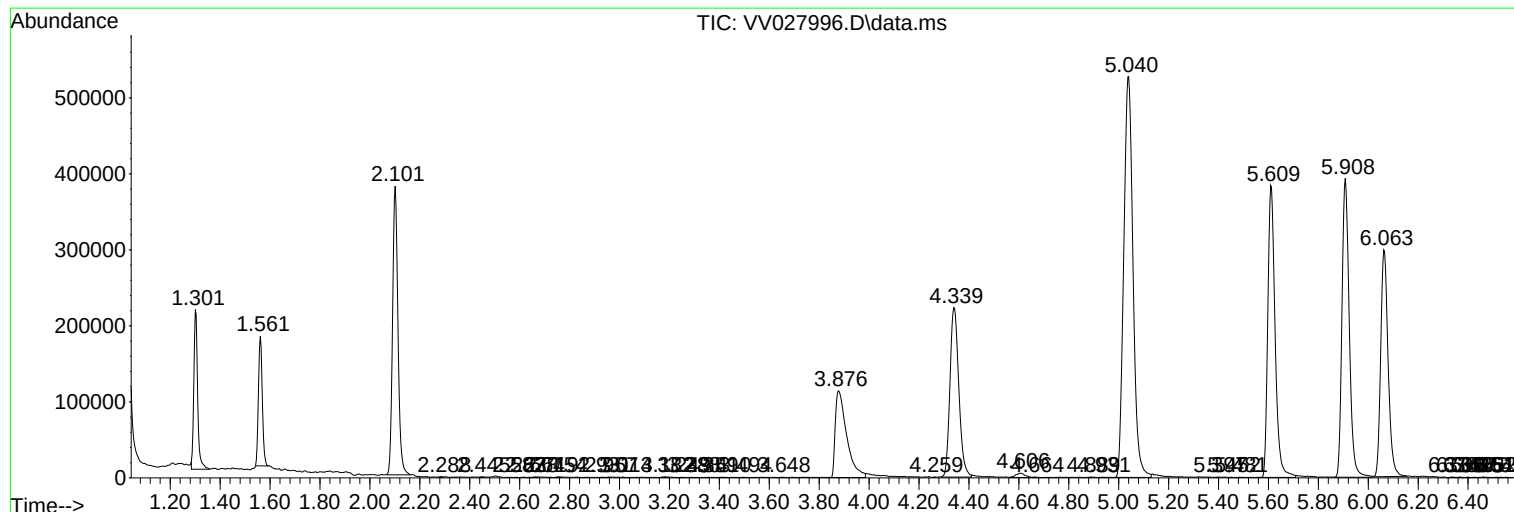

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027996.D
Acq On : 21 Sep 2022 05:32
Operator : SY/MD
Sample : N4674-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027996.D
Acq On : 21 Sep 2022 05:32
Operator : SY/MD
Sample : N4674-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc