

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027998.D
 Acq On : 21 Sep 2022 06:22
 Operator : SY/MD
 Sample : N4674-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	100	rVB	207609	221013	16.42%	1.978%
2	1.561	156	162	176	rVB	172474	191168	14.20%	1.711%
3	2.101	320	330	349	rBV	365392	540058	40.12%	4.833%
4	2.400	418	423	424	rBV2	314	280	0.02%	0.003%
5	2.545	466	468	471	rBV2	520	225	0.02%	0.002%
6	2.587	479	481	483	rBV2	376	207	0.02%	0.002%
7	2.632	490	495	497	rBV3	508	485	0.04%	0.004%
8	2.699	514	516	519	rBV	401	183	0.01%	0.002%
9	2.744	527	530	531	rBV2	491	230	0.02%	0.002%
10	2.822	551	554	556	rVB	399	232	0.02%	0.002%
11	2.841	556	560	561	rBV3	436	320	0.02%	0.003%
12	2.863	565	567	569	rVB	351	155	0.01%	0.001%
13	2.957	591	596	599	rBV4	676	513	0.04%	0.005%
14	2.979	599	603	607	rVB2	674	460	0.03%	0.004%
15	3.098	636	640	642	rBV2	211	157	0.01%	0.001%
16	3.140	652	653	658	rBV3	475	255	0.02%	0.002%
17	3.166	658	661	662	rBV2	524	286	0.02%	0.003%
18	3.233	680	682	684	rVB	361	159	0.01%	0.001%
19	3.265	687	692	695	rVB4	589	476	0.04%	0.004%
20	3.378	725	727	732	rVB2	373	243	0.02%	0.002%
21	3.404	732	735	737	rBV	286	192	0.01%	0.002%
22	3.429	741	743	747	rVB	280	174	0.01%	0.002%
23	3.468	752	755	758	rVB2	387	239	0.02%	0.002%
24	3.490	760	762	764	rVB2	408	182	0.01%	0.002%
25	3.529	770	774	781	rVB3	407	410	0.03%	0.004%
26	3.561	781	784	786	rBV	320	159	0.01%	0.001%
27	3.587	790	792	795	rVB	633	238	0.02%	0.002%
28	3.683	820	822	826	rBV	314	244	0.02%	0.002%
29	3.706	826	829	832	rVB2	240	155	0.01%	0.001%
30	3.883	873	884	923	rBV2	109748	368751	27.39%	3.300%
31	4.217	986	988	991	rBV3	529	218	0.02%	0.002%
32	4.339	1010	1026	1056	rBV	222425	553066	41.09%	4.949%
33	4.606	1095	1109	1123	rBV3	8952	21454	1.59%	0.192%
34	4.677	1129	1131	1135	rBV3	503	242	0.02%	0.002%
35	4.696	1135	1137	1139	rVB2	437	201	0.01%	0.002%
36	4.744	1150	1152	1154	rBV2	257	161	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027998.D
 Acq On : 21 Sep 2022 06:22
 Operator : SY/MD
 Sample : N4674-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	4.809	1168	1172	1176	rBV2	439	358	0.03%	0.003%
38	4.854	1183	1186	1188	rVV	691	325	0.02%	0.003%
39	4.876	1188	1193	1195	rVB2	485	281	0.02%	0.003%
40	4.934	1205	1211	1214	rVB5	477	424	0.03%	0.004%
41	5.040	1224	1244	1275	rBV2	521701	1346060	100.00%	12.046%
42	5.333	1332	1335	1336	rBV2	651	322	0.02%	0.003%
43	5.420	1360	1362	1366	rVB2	637	284	0.02%	0.003%
44	5.442	1366	1369	1372	rVB2	314	177	0.01%	0.002%
45	5.461	1372	1375	1379	rBV3	280	201	0.01%	0.002%
46	5.484	1381	1382	1384	rBV	391	180	0.01%	0.002%
47	5.510	1387	1390	1392	rBV3	336	176	0.01%	0.002%
48	5.522	1392	1394	1397	rBV3	364	214	0.02%	0.002%
49	5.545	1400	1401	1404	rVB3	427	173	0.01%	0.002%
50	5.564	1404	1407	1409	rBV2	576	266	0.02%	0.002%
51	5.609	1409	1421	1446	rBV	379983	766866	56.97%	6.863%
52	5.908	1501	1514	1548	rBV	296349	594814	44.19%	5.323%
53	6.063	1550	1562	1588	rVV	296038	600988	44.65%	5.378%
54	6.371	1655	1658	1659	rBV2	270	158	0.01%	0.001%
55	6.378	1659	1660	1664	rVB4	540	297	0.02%	0.003%
56	6.397	1664	1666	1670	rVB3	928	465	0.03%	0.004%
57	6.442	1674	1680	1684	rBV5	646	774	0.06%	0.007%
58	6.481	1688	1692	1696	rBV2	317	288	0.02%	0.003%
59	6.522	1701	1705	1706	rBV	391	306	0.02%	0.003%
60	6.982	1838	1848	1867	rBV	156354	287197	21.34%	2.570%
61	7.310	1939	1950	1969	rBV	621033	1080718	80.29%	9.671%
62	7.619	2037	2046	2071	rVB	113654	196953	14.63%	1.763%
63	7.847	2114	2117	2119	rBV2	1782	1039	0.08%	0.009%
64	8.011	2166	2168	2172	rVB2	943	492	0.04%	0.004%
65	8.085	2181	2191	2222	rBV	433406	806375	59.91%	7.216%
66	8.699	2379	2382	2384	rBV3	691	474	0.04%	0.004%
67	8.847	2417	2428	2449	rBV	609978	996781	74.05%	8.920%
68	9.101	2503	2507	2509	rBV3	1014	704	0.05%	0.006%
69	9.407	2600	2602	2603	rBV3	741	274	0.02%	0.002%
70	9.429	2607	2609	2610	rBV2	598	243	0.02%	0.002%
71	9.603	2661	2663	2667	rVB4	942	550	0.04%	0.005%
72	9.622	2667	2669	2670	rBV	547	221	0.02%	0.002%
73	9.715	2694	2698	2701	rBV4	622	595	0.04%	0.005%
74	9.841	2735	2737	2741	rBV2	892	700	0.05%	0.006%
75	9.918	2754	2761	2763	rBV4	830	919	0.07%	0.008%
76	9.956	2770	2773	2774	rBV2	508	321	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027998.D
 Acq On : 21 Sep 2022 06:22
 Operator : SY/MD
 Sample : N4674-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.117	2821	2823	2826	rBV3	1153	858	0.06%	0.008%
78	10.214	2840	2853	2866	rBV	475020	750483	55.75%	6.716%
79	10.500	2939	2942	2944	rBV3	492	345	0.03%	0.003%
80	10.525	2948	2950	2952	rBV2	640	332	0.02%	0.003%
81	10.567	2961	2963	2967	rBV4	801	665	0.05%	0.006%
82	10.677	2992	2997	3000	rBV5	1075	1109	0.08%	0.010%
83	10.715	3005	3009	3010	rBV3	506	278	0.02%	0.002%
84	10.818	3039	3041	3043	rBV2	533	302	0.02%	0.003%
85	10.853	3050	3052	3055	rBV2	628	336	0.02%	0.003%
86	10.889	3060	3063	3065	rBV2	691	541	0.04%	0.005%
87	10.950	3080	3082	3086	rBV3	558	436	0.03%	0.004%
88	11.040	3109	3110	3112	rBV2	634	255	0.02%	0.002%
89	11.175	3150	3152	3155	rBV3	510	241	0.02%	0.002%
90	11.246	3162	3174	3195	rBV	561605	861219	63.98%	7.707%
91	11.468	3241	3243	3248	rVB3	1009	721	0.05%	0.006%
92	11.535	3256	3264	3269	rBV7	5631	9891	0.73%	0.089%
93	11.622	3280	3291	3308	rBV	610377	950091	70.58%	8.502%
94	12.046	3421	3423	3424	rBV	573	218	0.02%	0.002%
95	12.352	3514	3518	3523	rBV6	1982	1990	0.15%	0.018%
96	12.763	3642	3646	3649	rBV3	662	533	0.04%	0.005%
97	12.831	3664	3667	3669	rBV	525	314	0.02%	0.003%
98	12.947	3701	3703	3707	rBV3	671	319	0.02%	0.003%
99	13.024	3724	3727	3730	rBV3	748	458	0.03%	0.004%
100	14.622	4222	4224	4225	rBV	755	401	0.03%	0.004%




Sum of corrected areas: 11174480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027998.D
Acq On : 21 Sep 2022 06:22
Operator : SY/MD
Sample : N4674-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

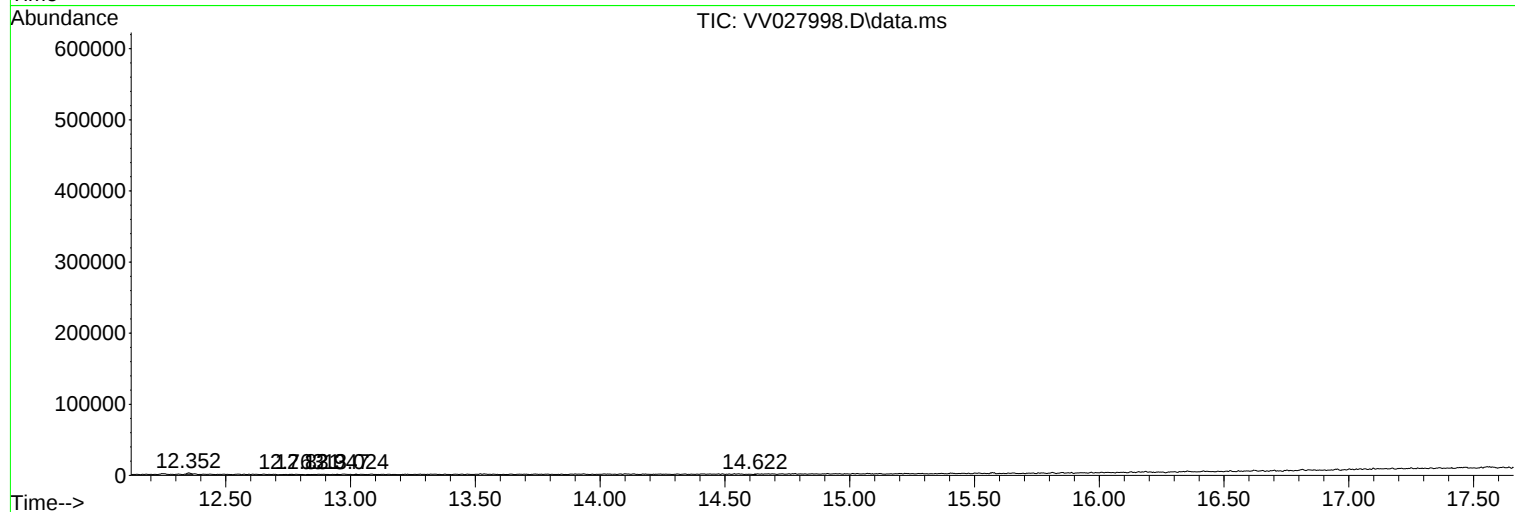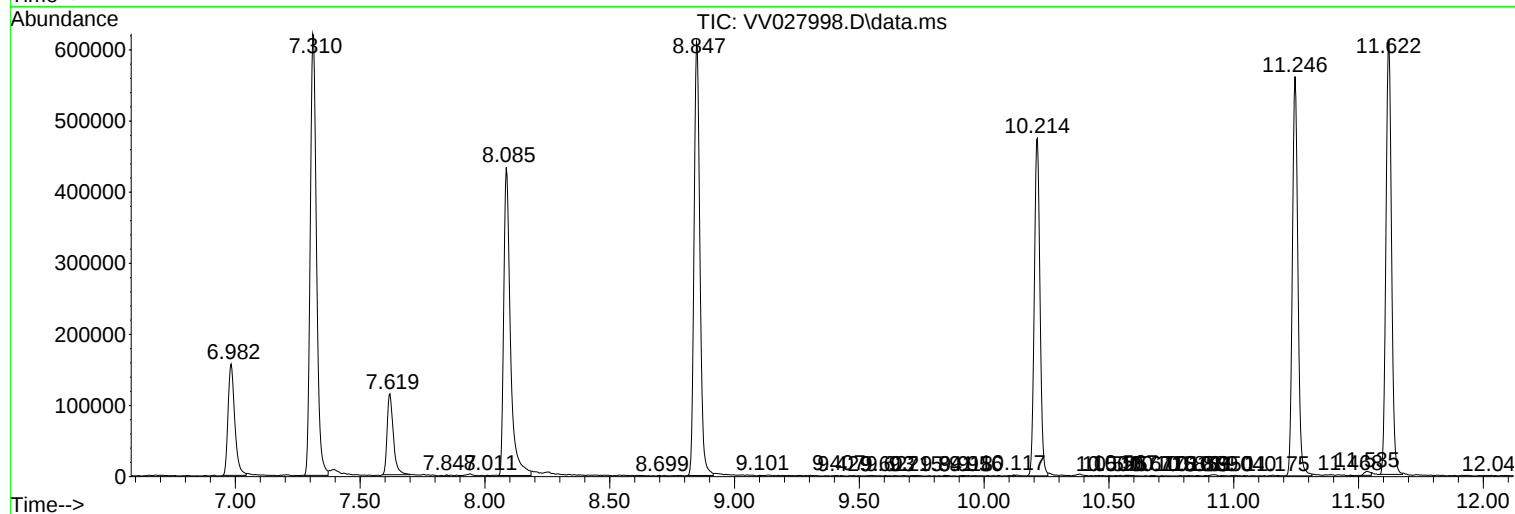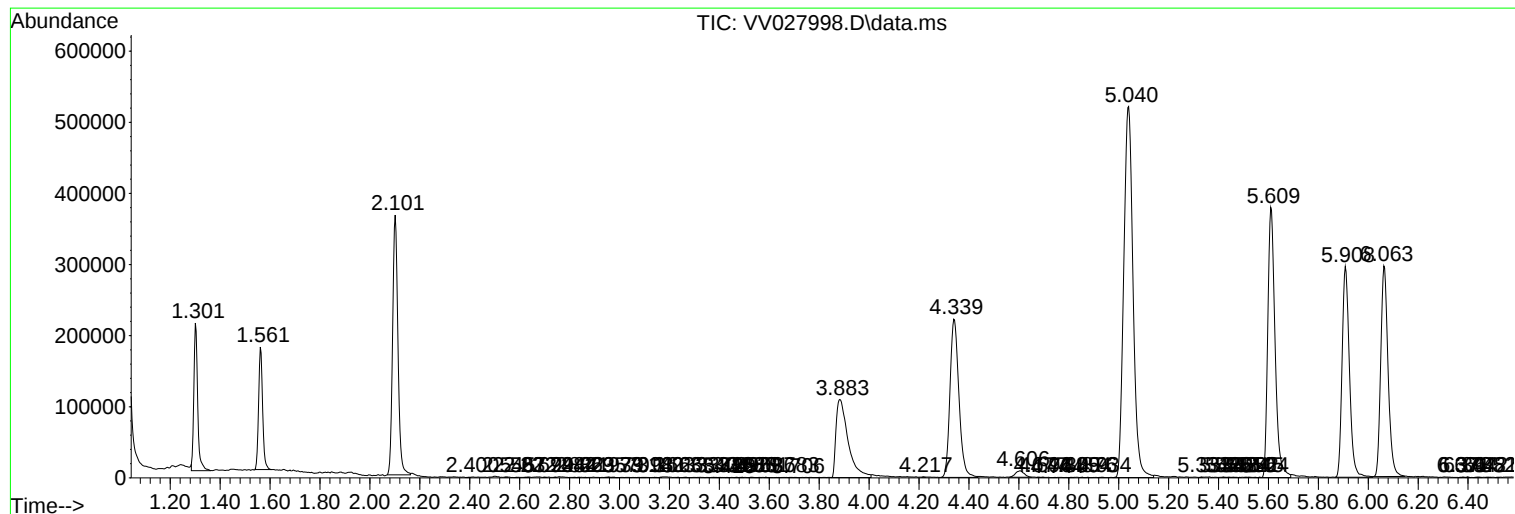

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027998.D
Acq On : 21 Sep 2022 06:22
Operator : SY/MD
Sample : N4674-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027998.D
Acq On : 21 Sep 2022 06:22
Operator : SY/MD
Sample : N4674-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc