

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV028000.D
 Acq On : 21 Sep 2022 07:11
 Operator : SY/MD
 Sample : N4674-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	209766	221558	9.21%	1.652%
2	1.561	156	162	177	rVB	167792	193632	8.05%	1.444%
3	2.102	320	330	348	rBV3	395678	629477	26.18%	4.695%
4	2.626	491	493	495	rBV	291	202	0.01%	0.002%
5	2.725	519	524	527	rBV5	699	667	0.03%	0.005%
6	2.757	529	534	537	rBV6	1384	1577	0.07%	0.012%
7	2.812	548	551	554	rBV	323	172	0.01%	0.001%
8	2.921	581	585	586	rBV	310	190	0.01%	0.001%
9	2.957	593	596	599	rBV2	716	366	0.02%	0.003%
10	2.979	600	603	606	rBV2	542	313	0.01%	0.002%
11	3.040	620	622	626	rVB2	368	193	0.01%	0.001%
12	3.069	626	631	632	rBV2	230	174	0.01%	0.001%
13	3.105	639	642	644	rBV2	406	195	0.01%	0.001%
14	3.124	644	648	650	rBV3	295	173	0.01%	0.001%
15	3.143	651	654	656	rVB	439	205	0.01%	0.002%
16	3.179	657	665	666	rBV3	1973	1728	0.07%	0.013%
17	3.349	717	718	721	rVB2	315	159	0.01%	0.001%
18	3.426	739	742	743	rBV	269	155	0.01%	0.001%
19	3.455	749	751	754	rVB	514	218	0.01%	0.002%
20	3.474	754	757	759	rBV2	305	189	0.01%	0.001%
21	3.513	765	769	774	rVB2	303	235	0.01%	0.002%
22	3.536	774	776	778	rVB	446	160	0.01%	0.001%
23	3.548	778	780	782	rBV2	463	220	0.01%	0.002%
24	3.706	824	829	835	rBV2	324	361	0.02%	0.003%
25	3.741	838	840	842	rVB	312	155	0.01%	0.001%
26	3.793	849	856	860	rBV4	504	444	0.02%	0.003%
27	3.812	860	862	865	rBV	503	336	0.01%	0.003%
28	3.844	870	872	874	rBV	313	178	0.01%	0.001%
29	3.892	874	887	925	rBV2	134619	475159	19.76%	3.544%
30	4.339	1011	1026	1053	rBV	226103	554691	23.07%	4.137%
31	4.603	1093	1108	1128	rVB2	38705	96777	4.03%	0.722%
32	4.738	1148	1150	1151	rBV2	367	165	0.01%	0.001%
33	4.754	1154	1155	1159	rVB2	500	247	0.01%	0.002%
34	4.786	1159	1165	1167	rBV3	526	520	0.02%	0.004%
35	4.822	1174	1176	1181	rVB3	653	398	0.02%	0.003%
36	4.899	1196	1200	1201	rBV3	259	201	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV028000.D
 Acq On : 21 Sep 2022 07:11
 Operator : SY/MD
 Sample : N4674-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.040	1226	1244	1272	rBV2	534167	1369257	56.95%	10.212%
38	5.420	1361	1362	1368	rVB2	715	316	0.01%	0.002%
39	5.529	1392	1396	1397	rBV	314	154	0.01%	0.001%
40	5.548	1400	1402	1405	rBV3	291	205	0.01%	0.002%
41	5.609	1409	1421	1448	rBV	376921	769830	32.02%	5.742%
42	5.815	1482	1485	1487	rBV4	605	327	0.01%	0.002%
43	5.844	1492	1494	1496	rBV	401	182	0.01%	0.001%
44	5.908	1499	1514	1547	rVV	1229798	2404379	100.00%	17.933%
45	6.063	1551	1562	1593	rVB	302508	622437	25.89%	4.642%
46	6.275	1626	1628	1631	rBV4	712	397	0.02%	0.003%
47	6.291	1631	1633	1636	rVB4	558	228	0.01%	0.002%
48	6.355	1651	1653	1658	rBV3	497	317	0.01%	0.002%
49	6.429	1674	1676	1680	rBV3	356	239	0.01%	0.002%
50	6.490	1694	1695	1697	rVB2	435	157	0.01%	0.001%
51	6.503	1697	1699	1701	rBV	270	173	0.01%	0.001%
52	6.571	1718	1720	1722	rVB	447	214	0.01%	0.002%
53	6.629	1736	1738	1740	rBV	514	224	0.01%	0.002%
54	6.744	1767	1774	1778	rBV5	294	470	0.02%	0.004%
55	6.764	1778	1780	1783	rVB2	482	219	0.01%	0.002%
56	6.783	1783	1786	1788	rBV2	571	375	0.02%	0.003%
57	6.825	1795	1799	1800	rBV	567	342	0.01%	0.003%
58	6.867	1811	1812	1816	rBV2	292	191	0.01%	0.001%
59	6.896	1816	1821	1827	rBV4	520	615	0.03%	0.005%
60	6.928	1829	1831	1832	rBV	426	164	0.01%	0.001%
61	6.982	1836	1848	1877	rBV2	160096	295924	12.31%	2.207%
62	7.310	1939	1950	1971	rBV	622969	1103254	45.89%	8.228%
63	7.619	2036	2046	2072	rBV	115661	211256	8.79%	1.576%
64	7.838	2112	2114	2117	rBV4	1574	1258	0.05%	0.009%
65	7.941	2138	2146	2155	rVB6	2911	4593	0.19%	0.034%
66	8.085	2181	2191	2227	rBV	450723	834308	34.70%	6.223%
67	8.555	2334	2337	2339	rBV2	846	557	0.02%	0.004%
68	8.847	2417	2428	2455	rBV	612525	1003166	41.72%	7.482%
69	9.313	2572	2573	2577	rVB3	826	428	0.02%	0.003%
70	9.336	2579	2580	2582	rVV2	573	204	0.01%	0.002%
71	9.375	2590	2592	2594	rBV2	635	394	0.02%	0.003%
72	9.564	2649	2651	2653	rVB3	784	256	0.01%	0.002%
73	9.603	2659	2663	2666	rBV3	737	694	0.03%	0.005%
74	9.625	2666	2670	2672	rBV3	848	603	0.03%	0.004%
75	9.776	2716	2717	2720	rBV	427	167	0.01%	0.001%
76	9.828	2730	2733	2736	rBV4	679	438	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV028000.D
 Acq On : 21 Sep 2022 07:11
 Operator : SY/MD
 Sample : N4674-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.924	2760	2763	2765	rBV3	666	473	0.02%	0.004%
78	9.957	2771	2773	2776	rBV	567	244	0.01%	0.002%
79	10.005	2787	2788	2790	rBV2	479	188	0.01%	0.001%
80	10.047	2798	2801	2803	rBV	566	341	0.01%	0.003%
81	10.069	2806	2808	2809	rBV	465	167	0.01%	0.001%
82	10.124	2817	2825	2834	rVB10	1777	3053	0.13%	0.023%
83	10.211	2840	2852	2871	rBV	480031	765865	31.85%	5.712%
84	10.577	2963	2966	2971	rBV4	1048	863	0.04%	0.006%
85	10.619	2977	2979	2981	rBV3	667	223	0.01%	0.002%
86	10.680	2993	2998	3000	rBV4	894	891	0.04%	0.007%
87	10.915	3065	3071	3075	rBV6	1800	2221	0.09%	0.017%
88	11.008	3099	3100	3102	rBV	415	178	0.01%	0.001%
89	11.034	3105	3108	3109	rBV3	457	264	0.01%	0.002%
90	11.143	3137	3142	3146	rBV6	1356	1282	0.05%	0.010%
91	11.198	3156	3159	3162	rBV3	614	393	0.02%	0.003%
92	11.246	3162	3174	3195	rBV	554131	855893	35.60%	6.384%
93	11.622	3279	3291	3310	rBV	612507	961091	39.97%	7.168%
94	12.014	3410	3413	3418	rBV4	915	750	0.03%	0.006%
95	12.606	3593	3597	3599	rBV3	1104	837	0.03%	0.006%
96	13.040	3730	3732	3733	rBV	689	225	0.01%	0.002%
97	13.082	3743	3745	3747	rBV3	748	398	0.02%	0.003%
98	13.320	3817	3819	3822	rBV2	670	356	0.01%	0.003%
99	13.480	3866	3869	3870	rBV2	637	423	0.02%	0.003%
100	13.773	3958	3960	3963	rBV	957	541	0.02%	0.004%




Sum of corrected areas: 13407862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV028000.D
Acq On : 21 Sep 2022 07:11
Operator : SY/MD
Sample : N4674-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

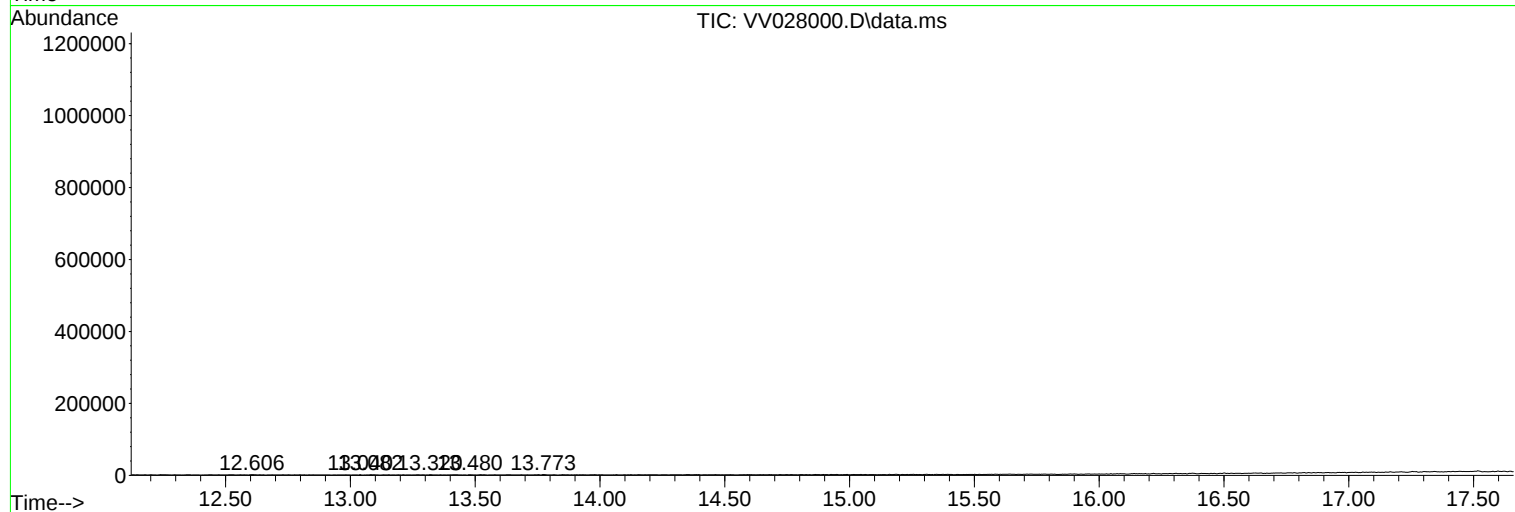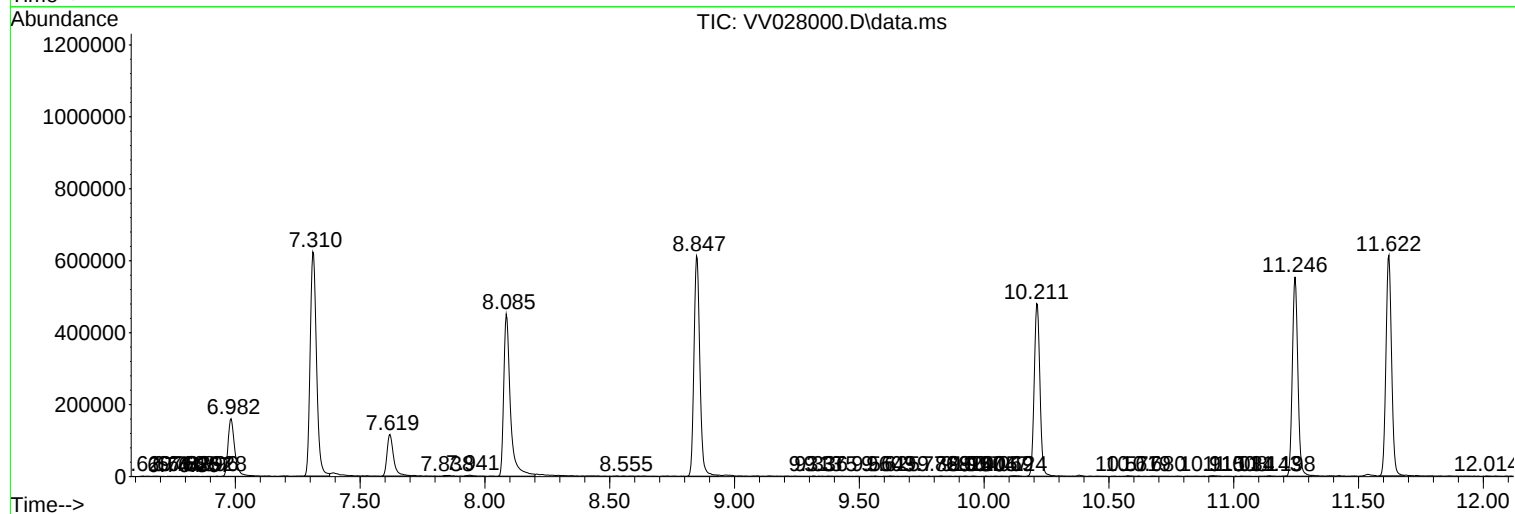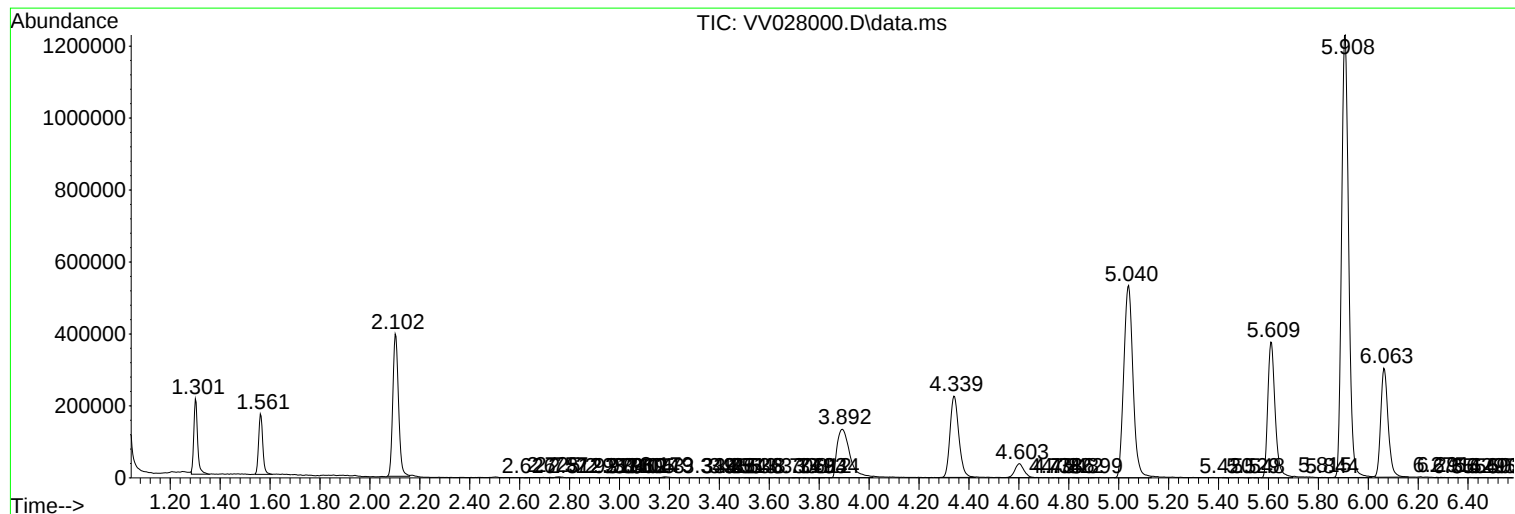

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV028000.D
Acq On : 21 Sep 2022 07:11
Operator : SY/MD
Sample : N4674-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV028000.D
Acq On : 21 Sep 2022 07:11
Operator : SY/MD
Sample : N4674-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc