

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV028001.D
 Acq On : 21 Sep 2022 07:35
 Operator : SY/MD
 Sample : N4674-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	103	rVB	207324	221139	15.07%	2.033%
2	1.561	156	162	179	rVB	165658	189475	12.91%	1.741%
3	2.102	320	330	353	rBV	348297	504136	34.35%	4.634%
4	2.378	414	416	423	rVB5	1011	954	0.07%	0.009%
5	2.597	482	484	485	rBV	667	258	0.02%	0.002%
6	2.754	530	533	534	rBV2	464	260	0.02%	0.002%
7	2.950	588	594	597	rBV4	1501	1599	0.11%	0.015%
8	3.143	651	654	661	rBV5	969	876	0.06%	0.008%
9	3.195	666	670	671	rBV2	686	406	0.03%	0.004%
10	3.249	683	687	691	rBV2	493	402	0.03%	0.004%
11	3.282	694	697	701	rBV3	521	330	0.02%	0.003%
12	3.423	735	741	742	rBV4	731	660	0.04%	0.006%
13	3.478	756	758	761	rVB2	807	444	0.03%	0.004%
14	3.507	764	767	771	rVB2	414	349	0.02%	0.003%
15	3.529	771	774	778	rBV	374	386	0.03%	0.004%
16	3.674	815	819	820	rBV	438	276	0.02%	0.003%
17	3.735	828	838	840	rBV3	549	766	0.05%	0.007%
18	3.883	874	884	929	rBV	113822	368151	25.09%	3.384%
19	4.339	1010	1026	1053	rBV	232490	571328	38.93%	5.251%
20	4.622	1110	1114	1116	rBV	483	403	0.03%	0.004%
21	4.687	1132	1134	1137	rVV2	668	323	0.02%	0.003%
22	4.745	1150	1152	1154	rBV2	570	277	0.02%	0.003%
23	4.835	1178	1180	1183	rVB4	502	296	0.02%	0.003%
24	4.899	1198	1200	1202	rBV2	651	266	0.02%	0.002%
25	5.040	1224	1244	1270	rBV2	575479	1467523	100.00%	13.488%
26	5.449	1367	1371	1373	rBV2	716	488	0.03%	0.004%
27	5.507	1384	1389	1392	rBV3	948	794	0.05%	0.007%
28	5.523	1392	1394	1396	rBV2	525	266	0.02%	0.002%
29	5.609	1410	1421	1455	rBV	404502	832617	56.74%	7.653%
30	5.912	1503	1515	1528	rBV	6783	15448	1.05%	0.142%
31	6.063	1550	1562	1585	rBV	328056	671027	45.73%	6.168%
32	6.359	1653	1654	1659	rVV2	552	407	0.03%	0.004%
33	6.388	1659	1663	1667	rVB3	689	566	0.04%	0.005%
34	6.416	1667	1672	1674	rBV3	339	280	0.02%	0.003%
35	6.461	1684	1686	1689	rBV	426	287	0.02%	0.003%
36	6.532	1706	1708	1712	rVB2	581	328	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV028001.D
 Acq On : 21 Sep 2022 07:35
 Operator : SY/MD
 Sample : N4674-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.577	1718	1722	1724	rBV2	654	521	0.04%	0.005%
38	6.658	1744	1747	1750	rBV3	522	308	0.02%	0.003%
39	6.770	1780	1782	1785	rVV	758	389	0.03%	0.004%
40	6.841	1796	1804	1806	rBV5	474	561	0.04%	0.005%
41	6.863	1807	1811	1812	rBV2	598	313	0.02%	0.003%
42	6.886	1815	1818	1819	rBV2	516	348	0.02%	0.003%
43	6.941	1832	1835	1837	rVV4	1196	573	0.04%	0.005%
44	6.982	1837	1848	1874	rBV2	158943	298025	20.31%	2.739%
45	7.310	1938	1950	1971	rBV	623402	1091689	74.39%	10.034%
46	7.619	2036	2046	2068	rBV	112216	202955	13.83%	1.865%
47	7.847	2114	2117	2119	rBV2	906	650	0.04%	0.006%
48	8.085	2179	2191	2233	rBV	431372	813217	55.41%	7.474%
49	8.461	2307	2308	2310	rBV2	945	343	0.02%	0.003%
50	8.773	2402	2405	2412	rVB4	727	564	0.04%	0.005%
51	8.847	2417	2428	2448	rBV	608658	1007966	68.68%	9.264%
52	9.143	2516	2520	2521	rBV3	765	487	0.03%	0.004%
53	9.220	2542	2544	2546	rBV3	597	286	0.02%	0.003%
54	9.326	2575	2577	2579	rBV	564	285	0.02%	0.003%
55	9.461	2616	2619	2622	rBV2	936	551	0.04%	0.005%
56	9.526	2637	2639	2641	rBV	439	264	0.02%	0.002%
57	9.596	2658	2661	2663	rBV3	514	279	0.02%	0.003%
58	9.719	2696	2699	2702	rVB	952	465	0.03%	0.004%
59	9.735	2702	2704	2706	rBV2	543	337	0.02%	0.003%
60	9.773	2712	2716	2718	rVB4	719	430	0.03%	0.004%
61	10.047	2798	2801	2803	rBV4	633	493	0.03%	0.005%
62	10.117	2818	2823	2824	rBV5	885	732	0.05%	0.007%
63	10.211	2841	2852	2874	rBV	470469	747836	50.96%	6.873%
64	10.346	2890	2894	2897	rBV4	692	534	0.04%	0.005%
65	10.545	2953	2956	2957	rBV2	626	339	0.02%	0.003%
66	10.593	2970	2971	2974	rBV3	602	285	0.02%	0.003%
67	10.612	2974	2977	2980	rBV2	570	366	0.02%	0.003%
68	10.651	2986	2989	2992	rBV5	523	363	0.02%	0.003%
69	10.667	2992	2994	2996	rBV	518	270	0.02%	0.002%
70	10.731	3011	3014	3017	rBV2	491	315	0.02%	0.003%
71	10.780	3027	3029	3034	rBV4	683	467	0.03%	0.004%
72	10.847	3048	3050	3052	rBV	528	275	0.02%	0.003%
73	10.870	3055	3057	3060	rVB3	641	251	0.02%	0.002%
74	11.034	3106	3108	3111	rBV2	673	447	0.03%	0.004%
75	11.108	3126	3131	3134	rBV3	692	601	0.04%	0.006%
76	11.137	3138	3140	3144	rVB3	857	505	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV028001.D
 Acq On : 21 Sep 2022 07:35
 Operator : SY/MD
 Sample : N4674-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.156	3144	3146	3148	rBV	722	259	0.02%	0.002%
78	11.198	3157	3159	3162	rBV4	559	317	0.02%	0.003%
79	11.246	3163	3174	3196	rBV	575985	876435	59.72%	8.055%
80	11.538	3259	3265	3276	rVB9	4380	6896	0.47%	0.063%
81	11.619	3279	3290	3314	rBV	602490	957149	65.22%	8.797%
82	12.043	3420	3422	3424	rBV3	651	374	0.03%	0.003%
83	12.149	3453	3455	3460	rVB4	528	266	0.02%	0.002%
84	12.217	3472	3476	3479	rBV2	515	428	0.03%	0.004%
85	12.233	3479	3481	3484	rBV3	726	555	0.04%	0.005%
86	12.320	3506	3508	3513	rVB3	865	618	0.04%	0.006%
87	12.368	3521	3523	3528	rBV5	990	810	0.06%	0.007%
88	12.416	3535	3538	3541	rBV3	698	476	0.03%	0.004%
89	12.513	3566	3568	3574	rVB3	796	543	0.04%	0.005%
90	12.567	3581	3585	3586	rBV3	534	345	0.02%	0.003%
91	12.628	3599	3604	3606	rBV3	781	736	0.05%	0.007%
92	12.828	3664	3666	3667	rBV2	672	317	0.02%	0.003%
93	13.133	3757	3761	3764	rVB4	938	584	0.04%	0.005%
94	13.365	3831	3833	3836	rBV	496	255	0.02%	0.002%
95	13.394	3839	3842	3845	rBV3	377	312	0.02%	0.003%
96	13.442	3853	3857	3861	rBV4	899	731	0.05%	0.007%
97	13.683	3928	3932	3935	rBV2	756	592	0.04%	0.005%
98	13.783	3960	3963	3966	rBV3	776	627	0.04%	0.006%
99	13.828	3975	3977	3979	rBV	527	300	0.02%	0.003%
100	14.294	4119	4122	4124	rBV3	583	418	0.03%	0.004%




Sum of corrected areas: 10880019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV028001.D
Acq On : 21 Sep 2022 07:35
Operator : SY/MD
Sample : N4674-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

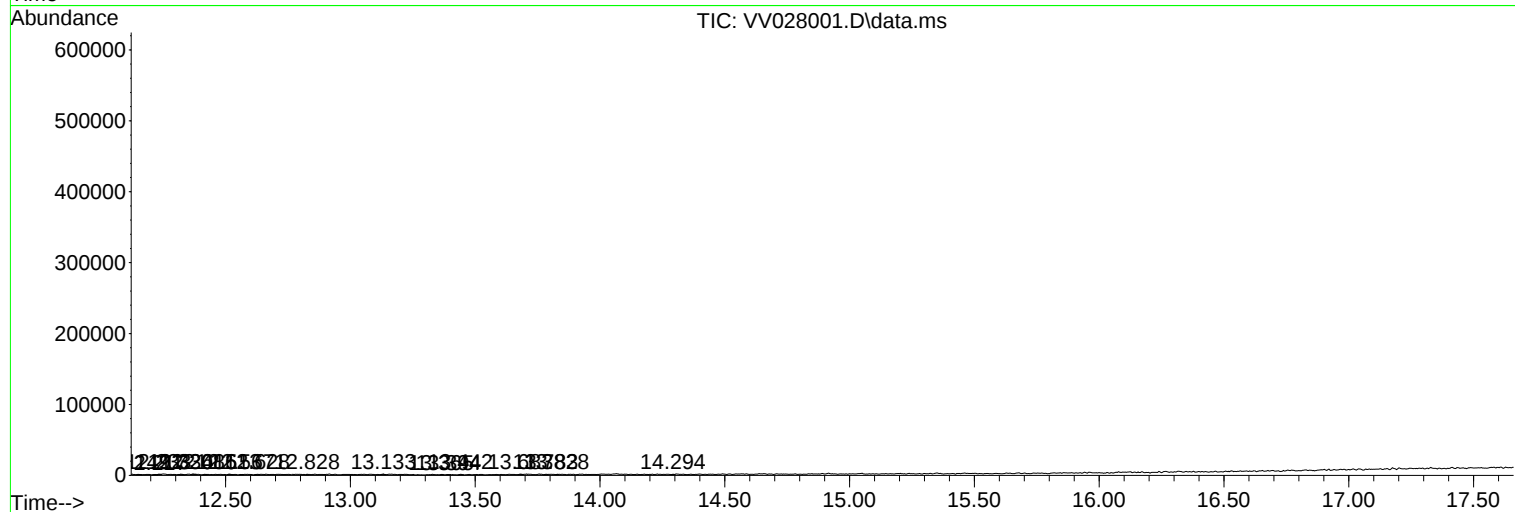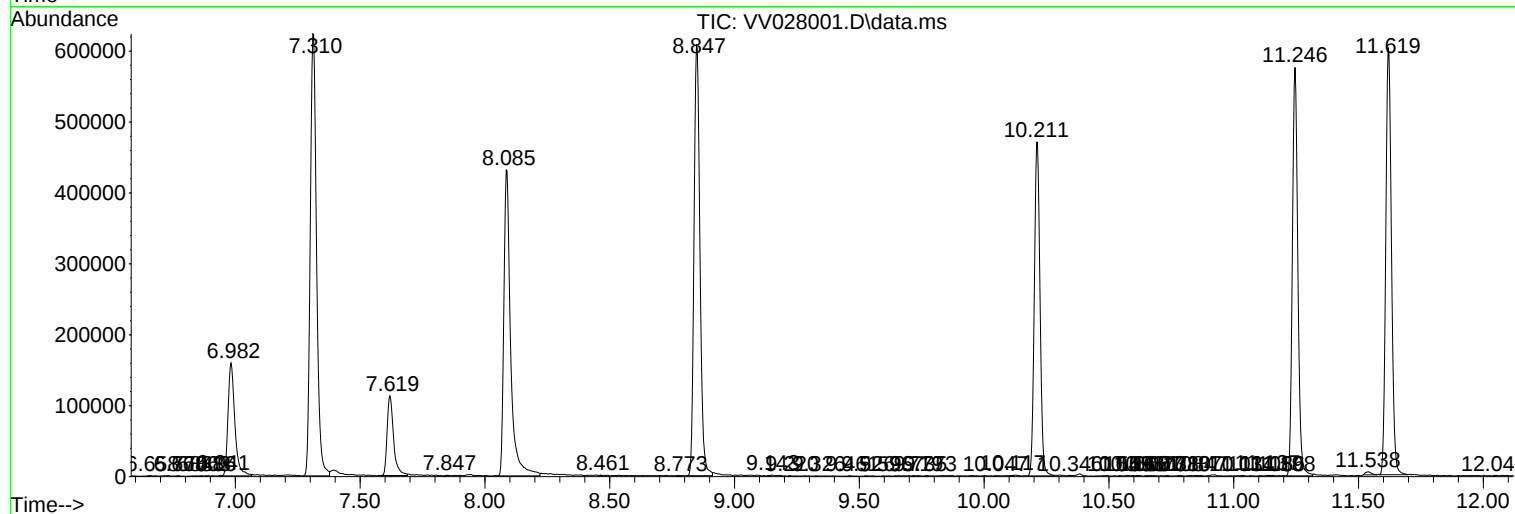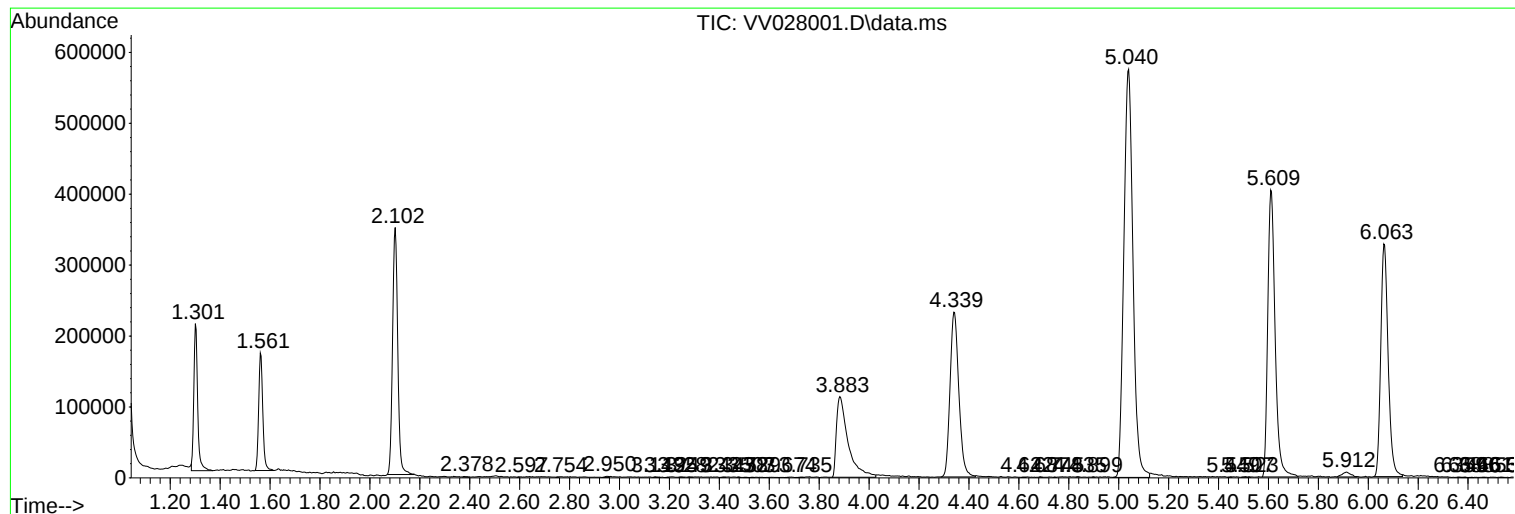

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV028001.D
Acq On : 21 Sep 2022 07:35
Operator : SY/MD
Sample : N4674-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV028001.D
Acq On : 21 Sep 2022 07:35
Operator : SY/MD
Sample : N4674-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------