
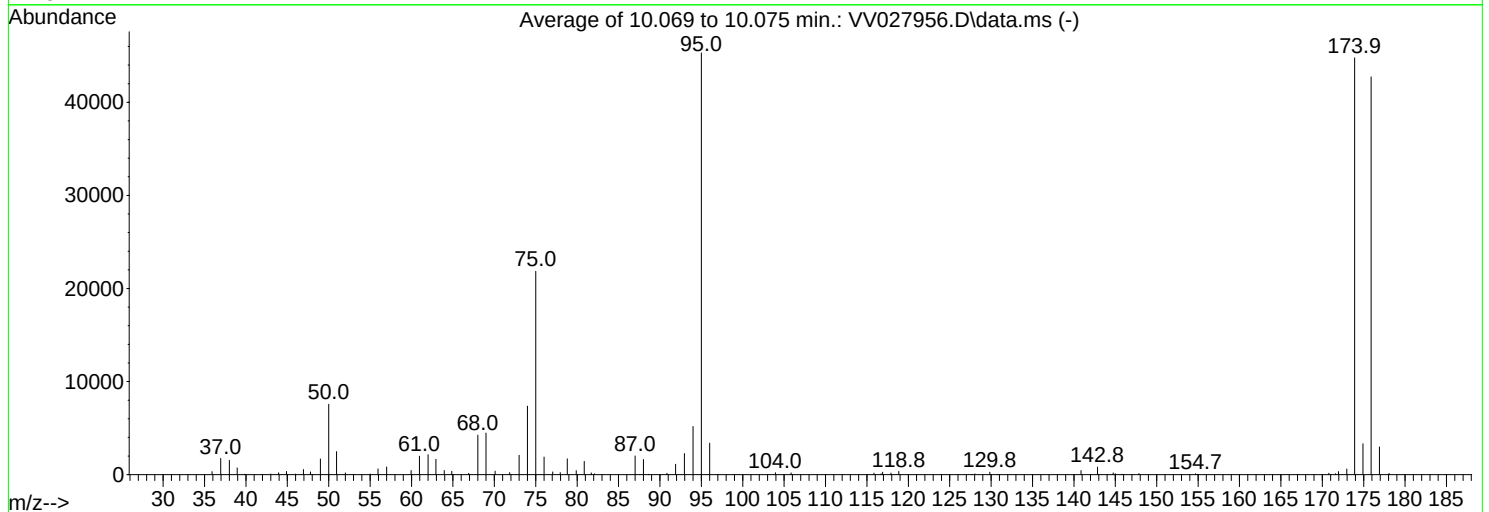


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027956.D
 Acq On : 20 Sep 2022 11:49
 Operator : SY/MD
 Sample : BFB320
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB320

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 22 05:25:17 2022

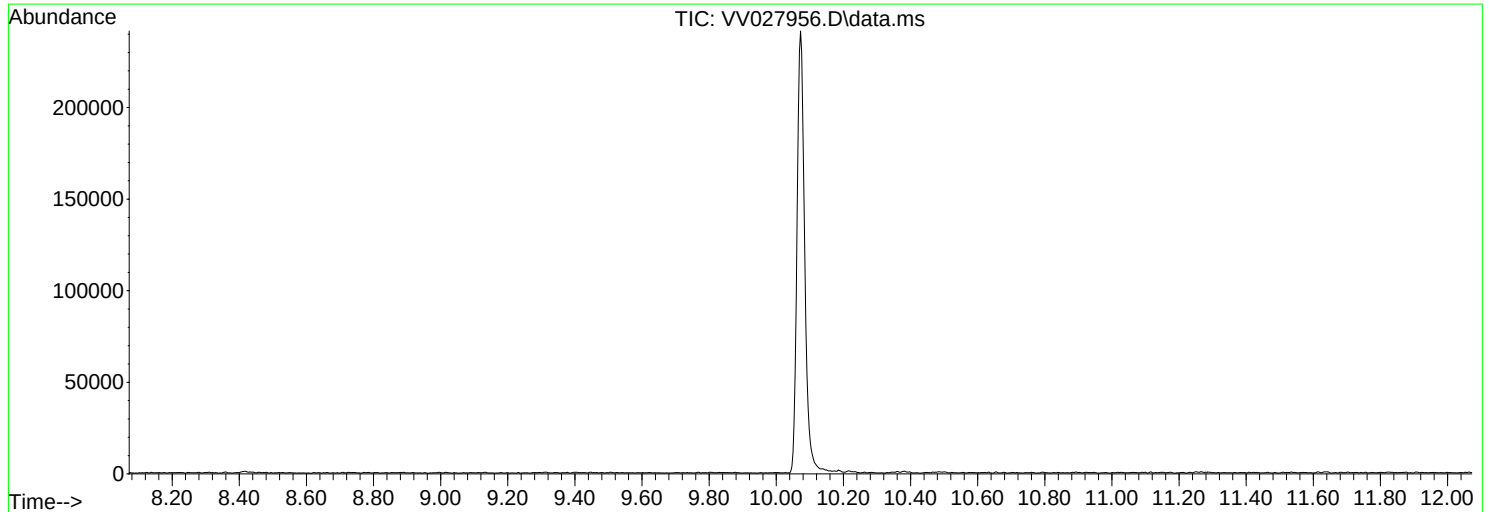

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	7561	PASS
75	95	30	80	48.2	21843	PASS
95	95	100	100	100.0	45315	PASS
96	95	5	9	7.5	3394	PASS
173	174	0.00	2	1.4	606	PASS
174	95	50	120	98.8	44773	PASS
175	174	5	9	7.4	3317	PASS
176	174	95	105	95.5	42736	PASS
177	176	5	10	6.9	2966	PASS

m/z	Abundance
39.90	268.0
44.00	243.0
57.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB320

m/z	Abundance
35.90	297.0
37.00	1702.0
38.00	1636.0
38.90	695.0
39.90	330.0
43.90	491.0
44.90	322.0
47.00	578.0
47.80	253.0
49.00	1528.0
50.00	7687.0
50.90	2463.0
52.00	151.0
56.00	654.0
57.10	790.0
59.90	409.0
60.90	2022.0
62.00	2031.0
63.00	1599.0
63.90	447.0
64.80	282.0
66.90	158.0
68.00	4404.0
69.00	4398.0
70.10	369.0
71.80	213.0
73.00	2139.0
74.00	7006.0
75.00	22432.0
76.00	1986.0
77.00	249.0
78.00	264.0
78.80	1703.0
80.00	379.0
80.80	1395.0
81.70	291.0
87.00	1901.0
88.00	1659.0
88.60	106.0
90.80	126.0
91.90	1010.0
93.00	2215.0
94.00	5099.0
95.00	44680.0
96.00	3361.0
97.00	124.0
104.00	239.0
105.90	191.0
115.90	166.0
116.70	275.0
116.90	274.0
117.90	163.0
118.80	308.0
127.70	120.0
129.80	207.0
140.90	340.0
142.90	742.0
144.70	287.0
145.70	111.0
147.90	128.0
154.70	170.0
170.80	159.0
171.90	321.0
173.00	621.0
173.90	43080.0
174.90	3156.0
175.90	41960.0
176.90	3048.0
178.10	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB320

m/z	Abundance
35.90	337.0
36.90	1787.0
38.00	1592.0
39.00	743.0
39.90	335.0
43.00	102.0
43.90	484.0
44.90	346.0
46.00	101.0
46.90	587.0
47.80	306.0
49.00	1759.0
50.00	7863.0
50.90	2535.0
52.00	200.0
55.00	101.0
55.90	653.0
57.00	810.0
60.00	455.0
60.90	2076.0
62.00	2288.0
63.00	1681.0
64.00	455.0
64.90	376.0
66.90	143.0
68.00	4334.0
69.00	4639.0
70.10	412.0
71.90	233.0
73.00	2181.0
74.00	7563.0
75.00	22744.0
76.00	1981.0
77.10	301.0
77.90	229.0
78.80	1727.0
79.90	436.0
80.80	1490.0
81.70	306.0
87.00	2055.0
88.00	1701.0
90.90	160.0
91.90	1164.0
93.00	2362.0
94.00	5381.0
95.00	46896.0
96.00	3477.0
104.00	207.0
105.80	178.0
115.90	173.0
116.90	246.0
117.90	180.0
118.90	357.0
128.10	117.0
129.90	254.0
140.80	467.0
142.90	853.0
144.80	284.0
147.80	135.0
154.70	148.0
170.80	172.0
172.00	345.0
172.90	595.0
173.90	46368.0
174.90	3416.0
175.90	44096.0
176.90	3133.0
178.00	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB320

m/z	Abundance
35.90	350.0
36.90	1706.0
38.00	1361.0
39.00	720.0
39.80	323.0
43.00	111.0
44.00	390.0
44.90	374.0
46.00	103.0
46.90	511.0
47.80	326.0
49.00	1779.0
50.00	7133.0
51.00	2411.0
52.00	197.0
55.00	110.0
55.90	573.0
56.90	853.0
60.00	468.0
61.00	1832.0
62.00	2118.0
62.90	1688.0
64.00	460.0
64.90	419.0
66.90	121.0
68.00	4016.0
69.00	4392.0
70.10	376.0
71.90	215.0
73.00	1902.0
74.00	7492.0
75.00	20352.0
76.00	1708.0
77.00	336.0
78.00	181.0
78.80	1665.0
79.80	488.0
80.90	1409.0
82.10	259.0
87.00	2057.0
88.00	1567.0
90.90	199.0
91.90	1208.0
92.90	2216.0
94.00	5051.0
95.00	44368.0
96.00	3344.0
103.90	157.0
105.80	182.0
115.80	189.0
116.90	275.0
117.90	182.0
118.90	345.0
128.00	116.0
129.80	289.0
130.80	115.0
140.80	532.0
142.80	852.0
145.00	314.0
145.90	108.0
147.80	113.0
154.90	123.0
170.80	133.0
171.60	320.0
172.00	299.0
172.90	603.0
173.90	44872.0
174.90	3378.0
175.90	42152.0
176.90	2717.0
178.00	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB320