




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028109.D
 Acq On : 23 Sep 2022 18:15
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:29:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 24 01:23:44 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/27/2022
 Supervised By :Mahesh Dadoda 09/27/2022

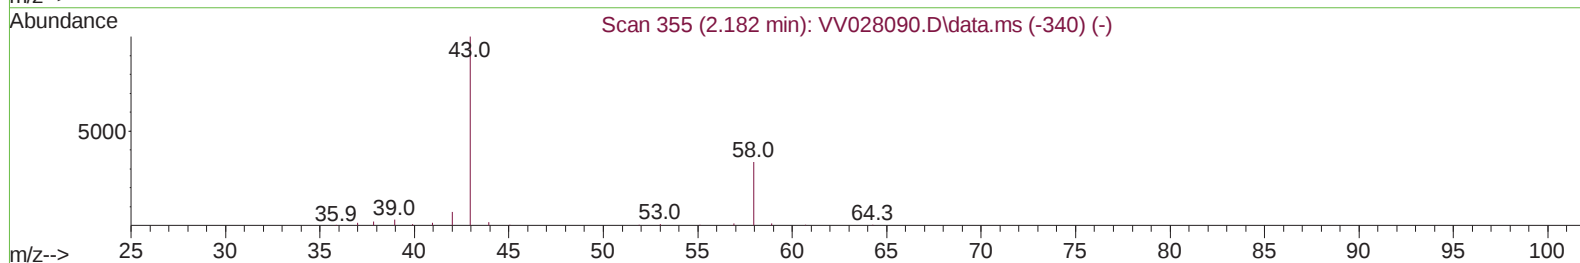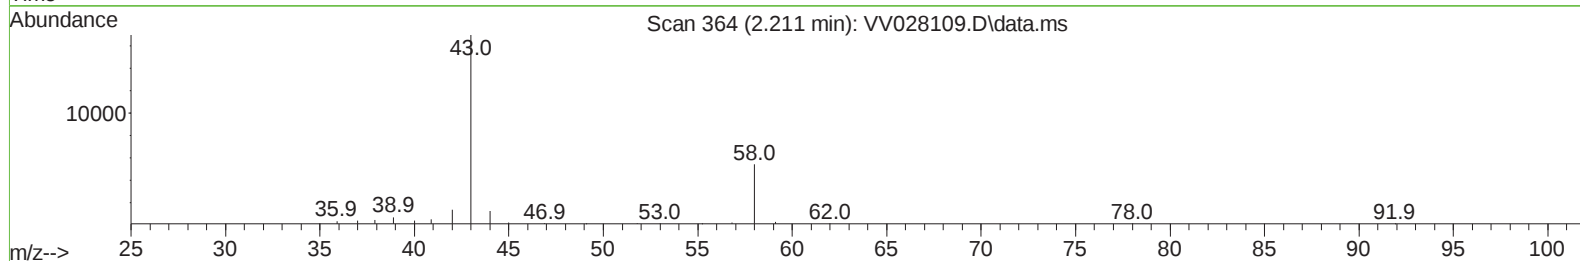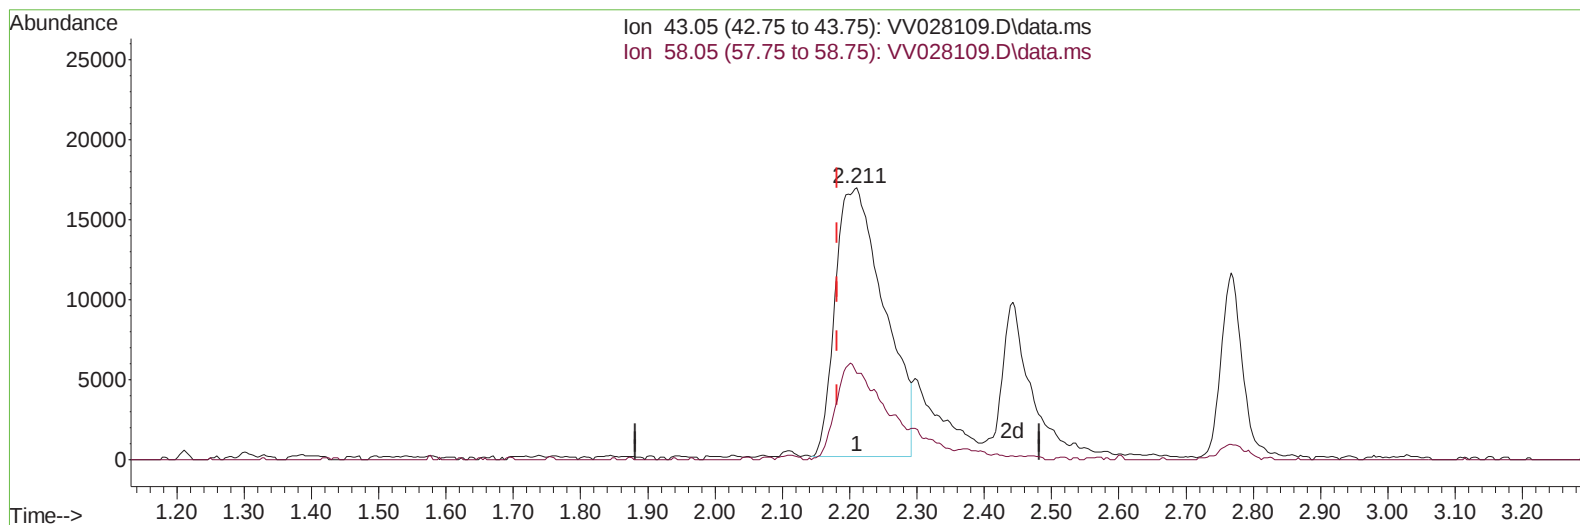

TIC: VV028109.D\data.ms

(13) Acetone (T)

2.211min (+ 0.029) 34.92 ug/L

response 84883

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	34.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028109.D
 Acq On : 23 Sep 2022 18:15
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:29:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 24 01:23:44 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/27/2022
 Supervised By :Mahesh Dadoda 09/27/2022

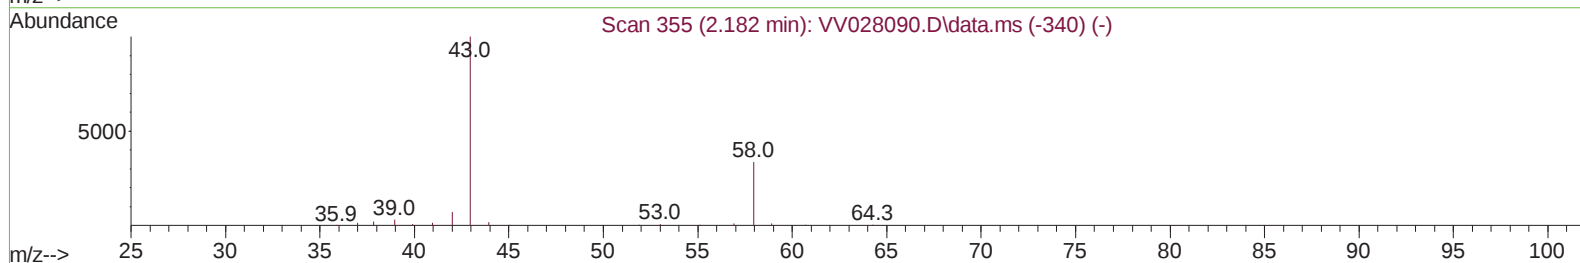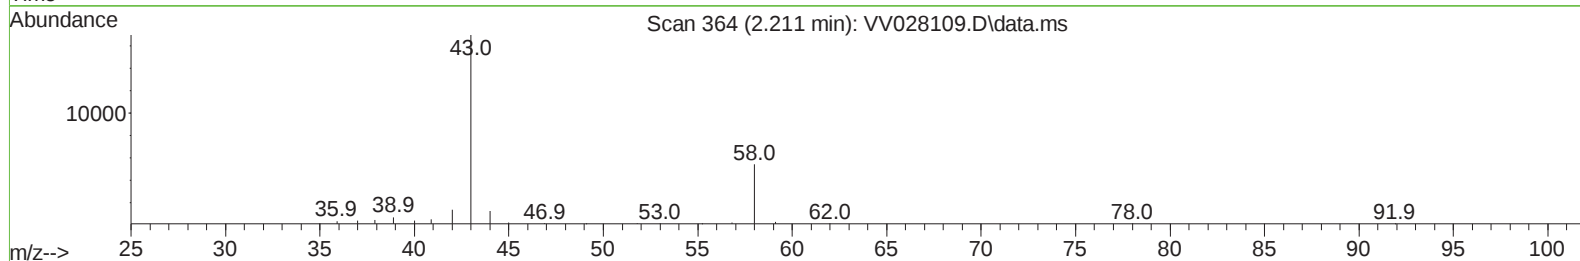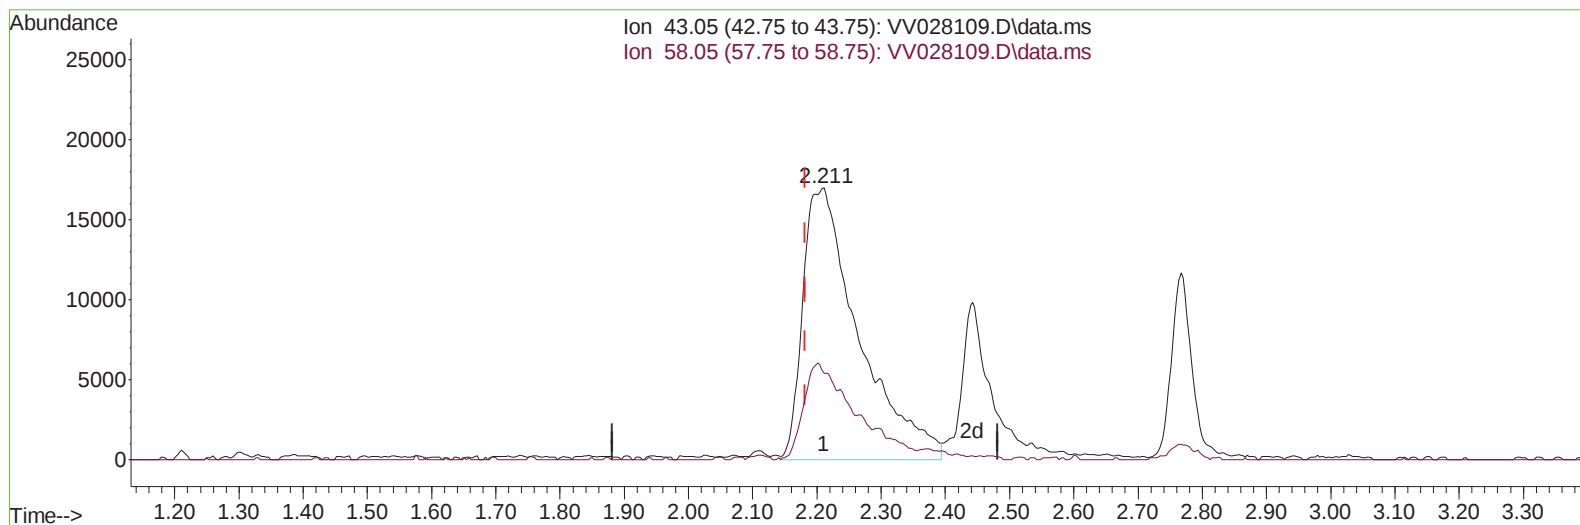

TIC: VV028109.D\data.ms

(13) Acetone (T)

2.211min (+ 0.029) 42.14 ug/L m

response 102425

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	28.34
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028109.D
 Acq On : 23 Sep 2022 18:15
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:29:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 24 01:23:44 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/27/2022
 Supervised By :Mahesh Dadoda 09/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	180282	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	181549	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	100575	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	74265	3.973	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	79.400%	
7) Chloroethane-d5	1.561	69	63495	4.273	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	85.400%	
11) 1,1-Dichloroethene-d2	2.101	63	128098	3.952	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	79.000%	
20) 2-Butanone-d5	3.905	46	171013	54.197	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	108.400%	
24) Chloroform-d	4.343	84	145747	4.887	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.027	65	69507	4.898	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	98.000%	
32) Benzene-d6	5.043	84	262004	4.401	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	88.000%	
36) 1,2-Dichloropropane-d6	6.066	67	84779	4.568	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	91.400%	
41) Toluene-d8	7.310	98	233436	4.332	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.600%	
43) trans-1,3-Dichloroprop...	7.619	79	30786	4.592	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	91.800%	
46) 2-Hexanone-d5	8.088	63	144660	51.704	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	103.400%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	63275	4.988	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	99.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	87660	4.444	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	88.800%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.124	85	65068	4.832	ug/L	94
3) Chloromethane	1.237	50	64315	3.607	ug/L	98
5) Vinyl chloride	1.304	62	70710	5.058	ug/L	99
6) Bromomethane	1.516	94	43613	4.790	ug/L	99
8) Chloroethane	1.577	64	44835	4.783	ug/L	99
9) Trichlorofluoromethane	1.748	101	108795	4.901	ug/L	97
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	62063	4.852	ug/L	98
12) 1,1-Dichloroethene	2.111	96	55350	4.443	ug/L	92
13) Acetone	2.211	43	102425m	42.142	ug/L	
14) Carbon disulfide	2.285	76	115675	4.838	ug/L	100
15) Methyl Acetate	2.442	43	22789	4.830	ug/L #	90
16) Methylene chloride	2.500	84	74248	5.339	ug/L	95
17) Methyl tert-butyl Ether	2.767	73	138763	5.177	ug/L	99
18) trans-1,2-Dichloroethene	2.754	96	56936	5.220	ug/L	99
19) 1,1-Dichloroethane	3.182	63	126651	5.323	ug/L	97
21) 2-Butanone	3.989	43	142191	47.255	ug/L	95
22) cis-1,2-Dichloroethene	3.905	96	64775	4.526	ug/L	98
23) Bromochloromethane	4.243	128	29833	5.206	ug/L	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028109.D
 Acq On : 23 Sep 2022 18:15
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:29:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 24 01:23:44 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/27/2022
 Supervised By :Mahesh Dadoda 09/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
25) Chloroform	4.368	83	134182	5.256	ug/L	99
27) 1,2-Dichloroethane	5.127	62	69550	5.109	ug/L #	94
29) 1,1,1-Trichloroethane	4.600	97	110701	4.963	ug/L	99
30) Cyclohexane	4.670	56	74530	4.620	ug/L	94
31) Carbon tetrachloride	4.822	117	93130	5.073	ug/L	99
33) Benzene	5.095	78	259372	5.145	ug/L	100
34) Trichloroethene	5.908	95	67454	5.375	ug/L	99
35) Methylcyclohexane	6.124	83	82167	4.774	ug/L	97
37) 1,2-Dichloropropane	6.169	63	69670	4.930	ug/L #	97
38) Bromodichloromethane	6.506	83	90863	5.207	ug/L	99
39) cis-1,3-Dichloropropene	7.024	75	87649	4.993	ug/L	98
40) 4-Methyl-2-pentanone	7.227	43	376707	54.888	ug/L	99
42) Toluene	7.384	91	277488	5.277	ug/L	98
44) trans-1,3-Dichloropropene	7.648	75	76871	5.091	ug/L	97
45) 1,1,2-Trichloroethane	7.834	97	48993	5.172	ug/L	97
47) Tetrachloroethene	7.973	164	50872	5.079	ug/L	95
48) 2-Hexanone	8.140	43	279727	53.689	ug/L	100
49) Dibromochloromethane	8.243	129	58622	5.146	ug/L	98
50) 1,2-Dibromoethane	8.352	107	43231	5.251	ug/L	97
51) Chlorobenzene	8.876	112	174610	4.950	ug/L	97
52) Ethylbenzene	9.008	91	278029	4.997	ug/L	99
53) m,p-Xylene	9.137	106	108811	5.104	ug/L	97
54) o-Xylene	9.542	106	106631	5.065	ug/L	100
55) Styrene	9.558	104	187652	5.144	ug/L	99
57) 1,1,2,2-Tetrachloroethane	10.239	83	58749	5.322	ug/L	99
59) Bromoform	9.728	173	31759	4.974	ug/L	99
60) Isopropylbenzene	9.927	105	285222	4.831	ug/L	99
61) 1,2,3-Trichloropropane	10.272	75	42784	5.072	ug/L	97
62) 1,3,5-Trimethylbenzene	10.535	105	75803	4.559	ug/L	99
63) 1,2,4-Trimethylbenzene	10.911	105	215039	4.626	ug/L	100
64) 1,3-Dichlorobenzene	11.178	146	145587	4.956	ug/L	99
65) 1,4-Dichlorobenzene	11.268	146	145284	4.943	ug/L	99
67) 1,2-Dichlorobenzene	11.641	146	136594	4.922	ug/L	98
68) 1,2-Dibromo-3-chloropr...	12.423	75	9575	5.178	ug/L	88
69) 1,3,5-Trichlorobenzene	12.641	180	111064	4.777	ug/L	99
70) 1,2,4-trichlorobenzene	13.259	180	86738	4.665	ug/L	100
71) Naphthalene	13.500	128	137461	4.514	ug/L	99
72) 1,2,3-Trichlorobenzene	13.741	180	81075	4.820	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:29:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 24 01:23:44 2022
Response via : Initial Calibration

