

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028099.D
 Acq On : 23 Sep 2022 13:25
 Operator : SY/MD
 Sample : N4652-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 24 01:27:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 24 01:23:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	192864	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	189453	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	90043	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	81280	4.065	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.400%
7) Chloroethane-d5	1.564	69	69642	4.381	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.600%
11) 1,1-Dichloroethene-d2	2.101	63	109406	3.155	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.000%
20) 2-Butanone-d5	3.899	46	154318	45.716	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.440%
24) Chloroform-d	4.342	84	139845	4.383	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.030	65	69608	4.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
32) Benzene-d6	5.043	84	262258	4.222	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
36) 1,2-Dichloropropane-d6	6.066	67	83351	4.304	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.000%
41) Toluene-d8	7.313	98	209162	3.720	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.400%
43) trans-1,3-Dichloroprop...	7.622	79	27682	3.957	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.088	63	125179	42.875	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.740%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	60049	4.536	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	84403	4.779	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds						
16) Methylene chloride	2.500	84	4925	0.331	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028099.D
Acq On : 23 Sep 2022 13:25
Operator : SY/MD
Sample : N4652-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Sep 24 01:27:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 24 01:23:44 2022
Response via : Initial Calibration

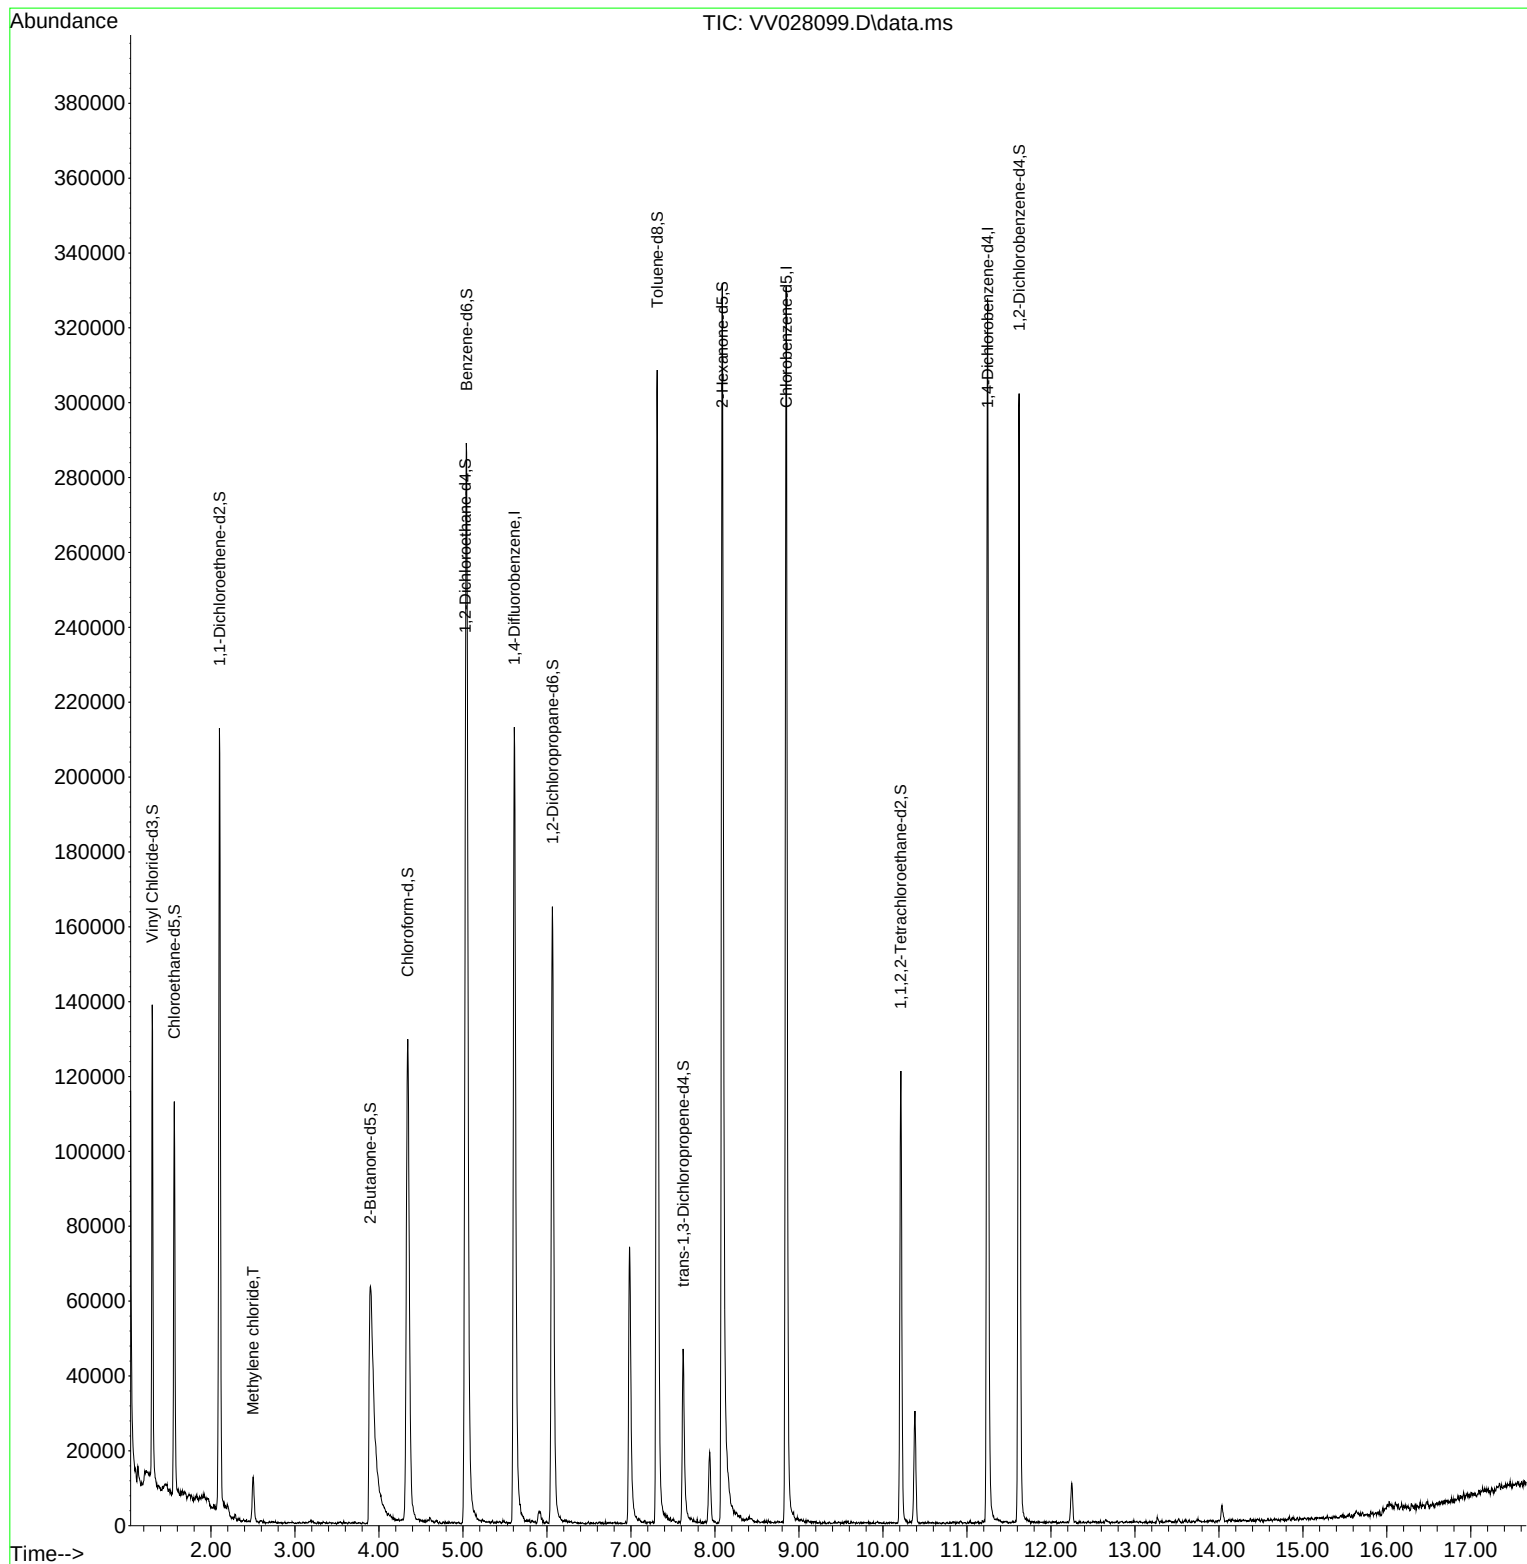

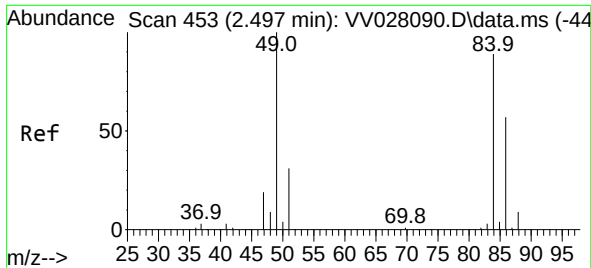

#16
Methylene chloride
Concen: 0.331 ug/L
RT: 2.500 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV028099.D
Acq: 23 Sep 2022 13:25

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 4925
Ion Ratio Lower Upper
84 100
86 65.8 46.8 86.8
49 113.5 87.5 162.5

