

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028091.D
 Acq On : 23 Sep 2022 10:07
 Operator : SY/MD
 Sample : VV0923WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK234

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	93	rVB	145308	145158	19.28%	2.392%
2	1.561	154	162	172	rBV	119912	136712	18.16%	2.253%
3	2.098	319	329	348	rVB	225854	330609	43.91%	5.449%
4	2.497	441	453	464	rBV5	6501	11524	1.53%	0.190%
5	3.876	872	882	918	rBV	82436	261838	34.78%	4.316%
6	4.336	1009	1025	1051	rBV	137613	344572	45.77%	5.679%
7	5.037	1227	1243	1270	rBV3	298302	752911	100.00%	12.409%
8	5.609	1408	1421	1448	rBV	204426	426763	56.68%	7.034%
9	6.063	1549	1562	1583	rBV	179139	371951	49.40%	6.130%
10	6.982	1835	1848	1872	rBV	82022	157774	20.96%	2.600%
11	7.310	1938	1950	1971	rBV	323184	582666	77.39%	9.603%
12	7.619	2038	2046	2071	rBV2	47766	92570	12.29%	1.526%
13	8.085	2181	2191	2226	rBV	344622	687612	91.33%	11.333%
14	8.847	2416	2428	2449	rBV	327686	547470	72.71%	9.023%
15	10.210	2840	2852	2871	rBV	125014	208365	27.67%	3.434%
16	11.246	3163	3174	3201	rBV	311444	488950	64.94%	8.059%
17	11.622	3280	3291	3306	rBV	304098	497510	66.08%	8.200%
18	15.924	4618	4629	4630	rBV7	14697	22393	2.97%	0.369%




Sum of corrected areas: 6067348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028091.D
Acq On : 23 Sep 2022 10:07
Operator : SY/MD
Sample : VV0923WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

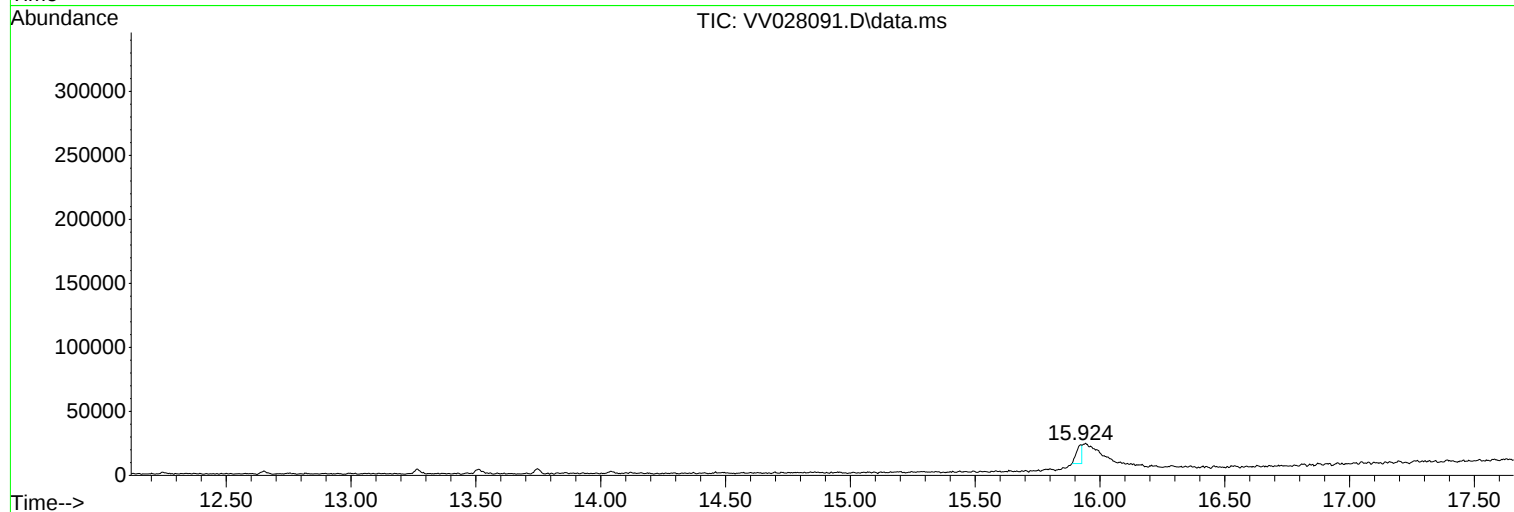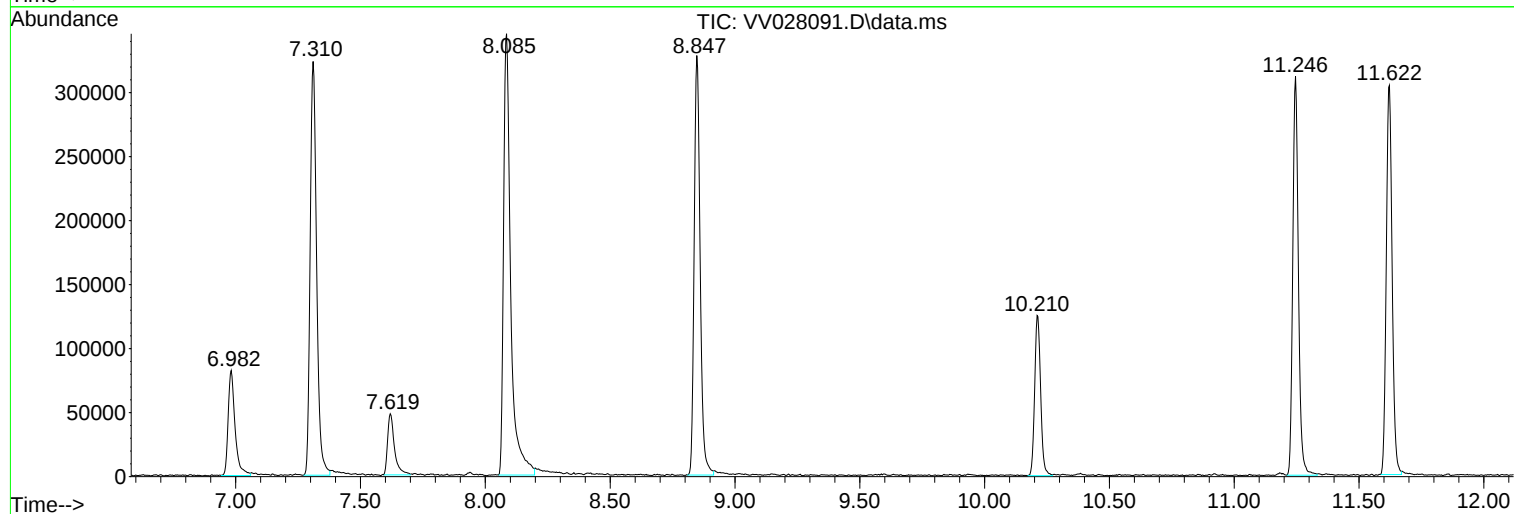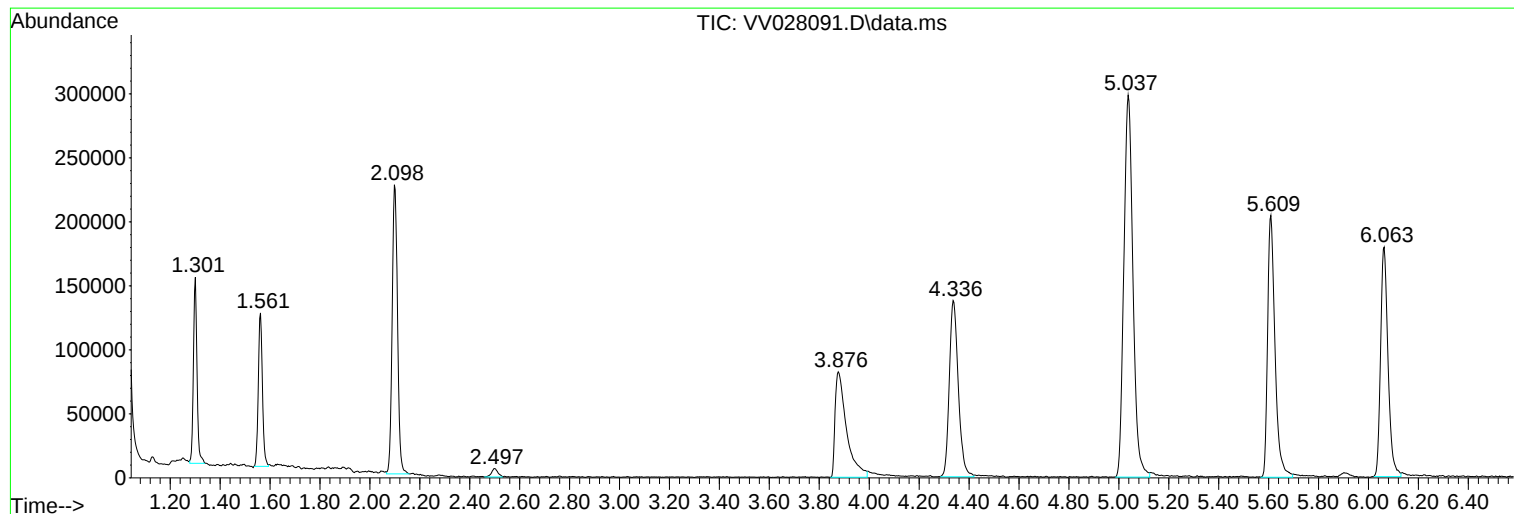

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028091.D
Acq On : 23 Sep 2022 10:07
Operator : SY/MD
Sample : VV0923WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028091.D
Acq On : 23 Sep 2022 10:07
Operator : SY/MD
Sample : VV0923WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
