

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028093.D
 Acq On : 23 Sep 2022 10:59
 Operator : SY/MD
 Sample : N4621-13 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8J8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	24	28	36	rVB2	6329	7905	1.13%	0.134%
2	1.301	75	81	96	rVB	136916	142137	20.30%	2.403%
3	1.561	154	162	179	rBV	107557	127718	18.24%	2.159%
4	2.101	319	330	347	rBV	214250	311095	44.44%	5.259%
5	2.503	443	455	465	rBV	7609	12098	1.73%	0.205%
6	3.902	879	890	933	rBV2	60731	275621	39.37%	4.659%
7	4.343	1009	1027	1053	rBV	126807	323904	46.27%	5.476%
8	5.040	1229	1244	1270	rBV2	279786	700074	100.00%	11.835%
9	5.613	1409	1422	1442	rBV	206112	422613	60.37%	7.144%
10	6.066	1548	1563	1596	rBV	163973	345901	49.41%	5.847%
11	6.982	1838	1848	1869	rBV	72997	142274	20.32%	2.405%
12	7.313	1939	1951	1973	rBV	294305	530034	75.71%	8.960%
13	7.622	2037	2047	2067	rBV2	44779	84262	12.04%	1.424%
14	8.088	2181	2192	2229	rBV	323415	651370	93.04%	11.011%
15	8.850	2413	2429	2461	rBV2	332245	635697	90.80%	10.746%
16	10.214	2841	2853	2867	rBV	121010	192060	27.43%	3.247%
17	11.246	3163	3174	3197	rBV	312250	502933	71.84%	8.502%
18	11.529	3253	3262	3274	rVB2	16385	26751	3.82%	0.452%
19	11.622	3277	3291	3310	rBV	299609	480940	68.70%	8.130%




Sum of corrected areas: 5915387

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028093.D
Acq On : 23 Sep 2022 10:59
Operator : SY/MD
Sample : N4621-13 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

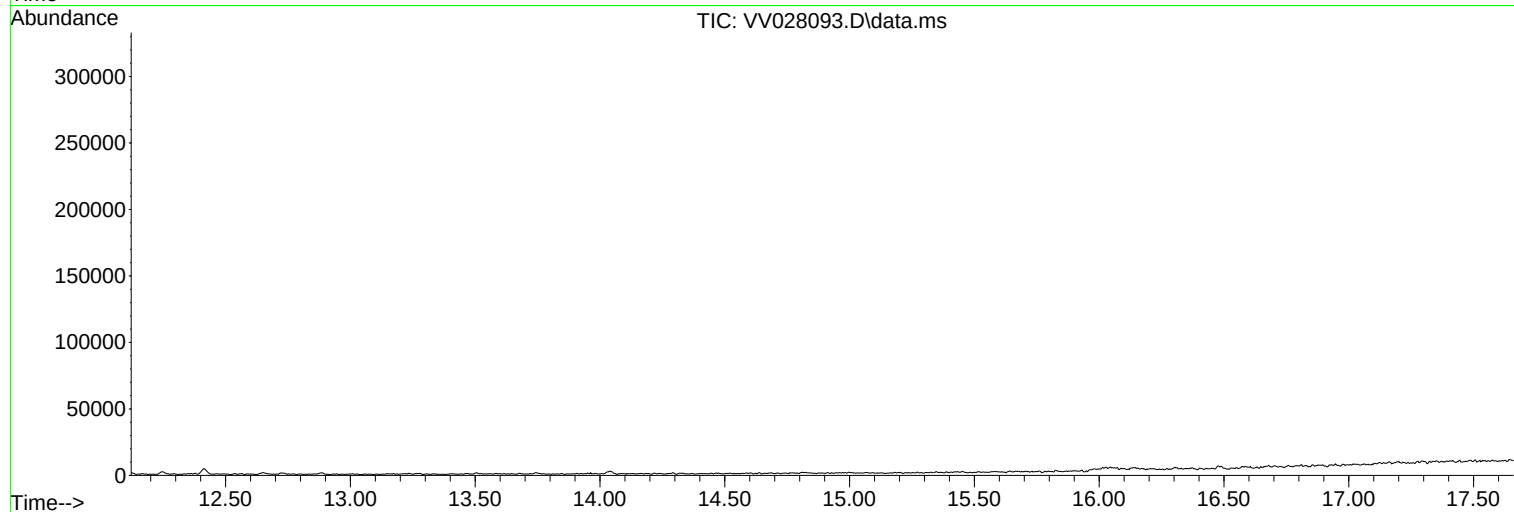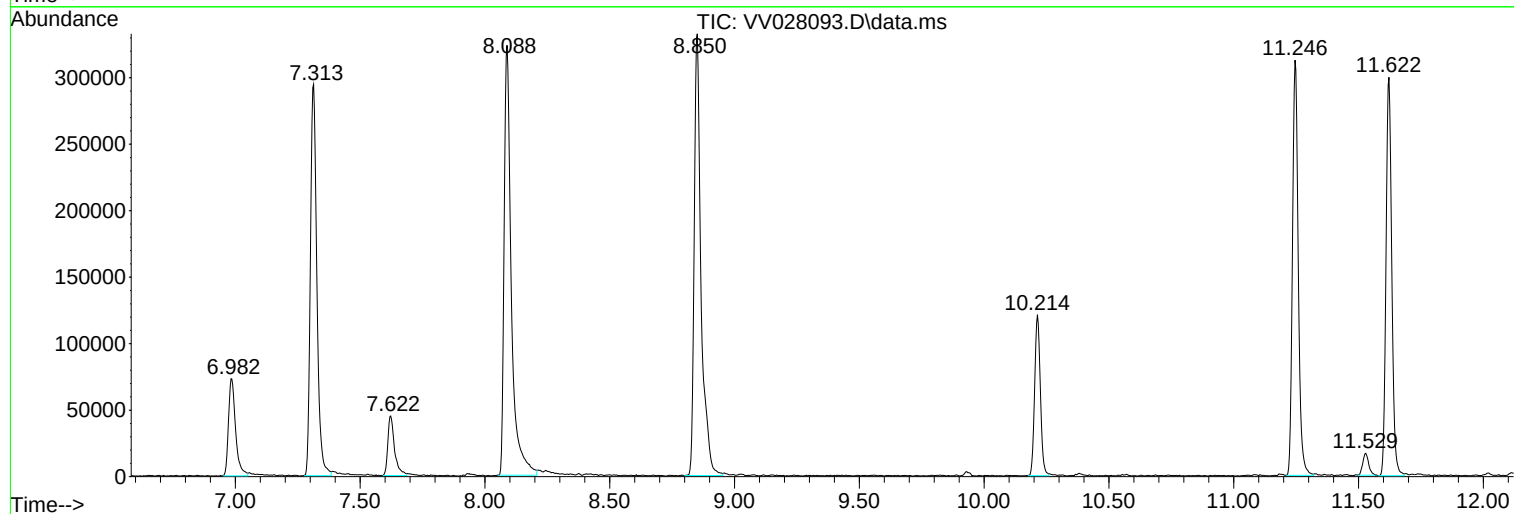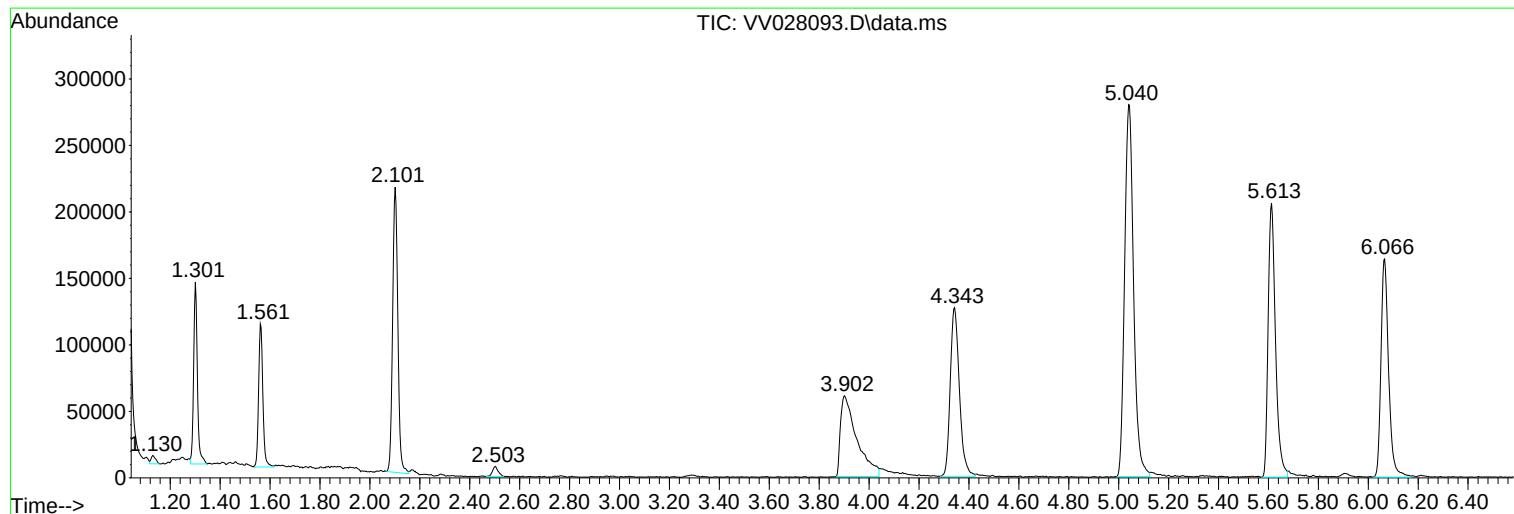

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028093.D
Acq On : 23 Sep 2022 10:59
Operator : SY/MD
Sample : N4621-13 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028093.D
Acq On : 23 Sep 2022 10:59
Operator : SY/MD
Sample : N4621-13 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc