

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028094.D
 Acq On : 23 Sep 2022 11:24
 Operator : SY/MD
 Sample : N4729-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXFJ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	94	rVB	137808	142392	19.71%	2.422%
2	1.561	155	162	173	rBV	109831	125777	17.41%	2.140%
3	2.101	320	330	349	rBV	220704	313545	43.40%	5.334%
4	3.895	878	888	931	rBV	63975	259558	35.92%	4.416%
5	4.342	1011	1027	1059	rBV	135879	352442	48.78%	5.996%
6	5.040	1227	1244	1274	rBV3	289215	722511	100.00%	12.291%
7	5.612	1410	1422	1452	rBV	203203	424503	58.75%	7.222%
8	5.911	1504	1515	1525	rBV9	4418	10337	1.43%	0.176%
9	6.066	1550	1563	1587	rBV	165844	349123	48.32%	5.939%
10	6.985	1838	1849	1871	rBV	73251	143668	19.88%	2.444%
11	7.313	1937	1951	1969	rBV	306343	540316	74.78%	9.192%
12	7.622	2038	2047	2068	rBV2	45190	85273	11.80%	1.451%
13	8.088	2181	2192	2235	rBV	324446	653116	90.40%	11.111%
14	8.850	2417	2429	2461	rBV	324241	540532	74.81%	9.196%
15	10.213	2840	2853	2870	rBV	118646	188474	26.09%	3.206%
16	10.381	2895	2905	2919	rVB3	12181	20229	2.80%	0.344%
17	11.246	3162	3174	3195	rBV	313406	488194	67.57%	8.305%
18	11.532	3253	3263	3276	rBV3	15165	30341	4.20%	0.516%
19	11.622	3280	3291	3311	rVV	304557	487875	67.52%	8.300%




Sum of corrected areas: 5878206

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028094.D
Acq On : 23 Sep 2022 11:24
Operator : SY/MD
Sample : N4729-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

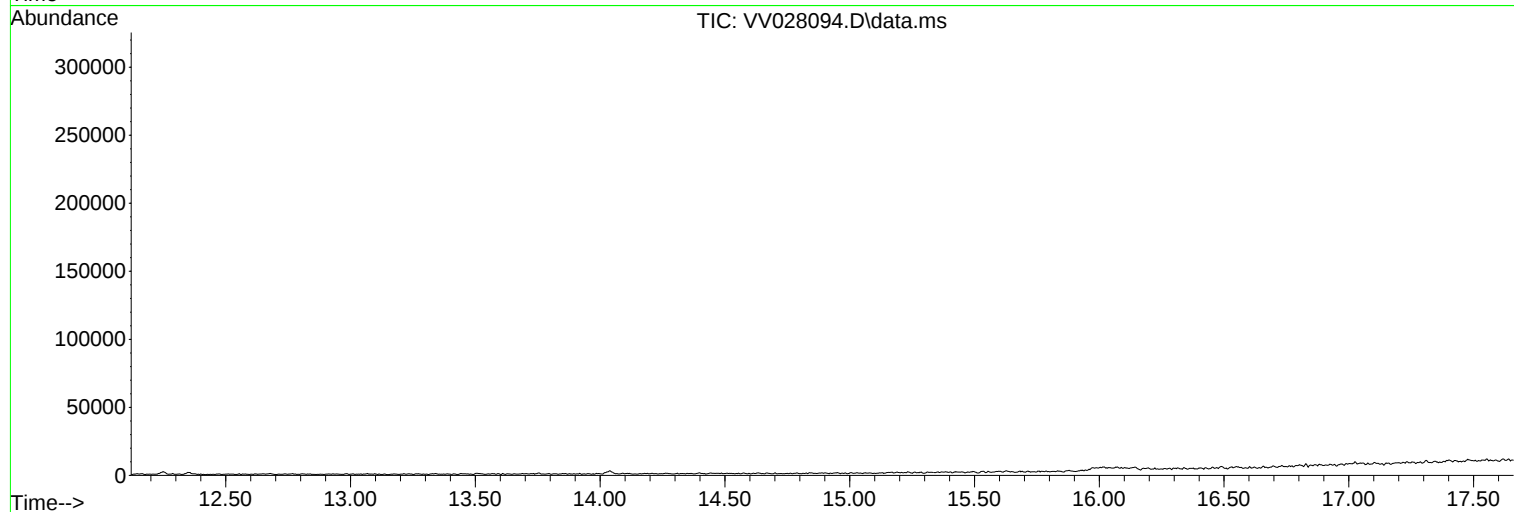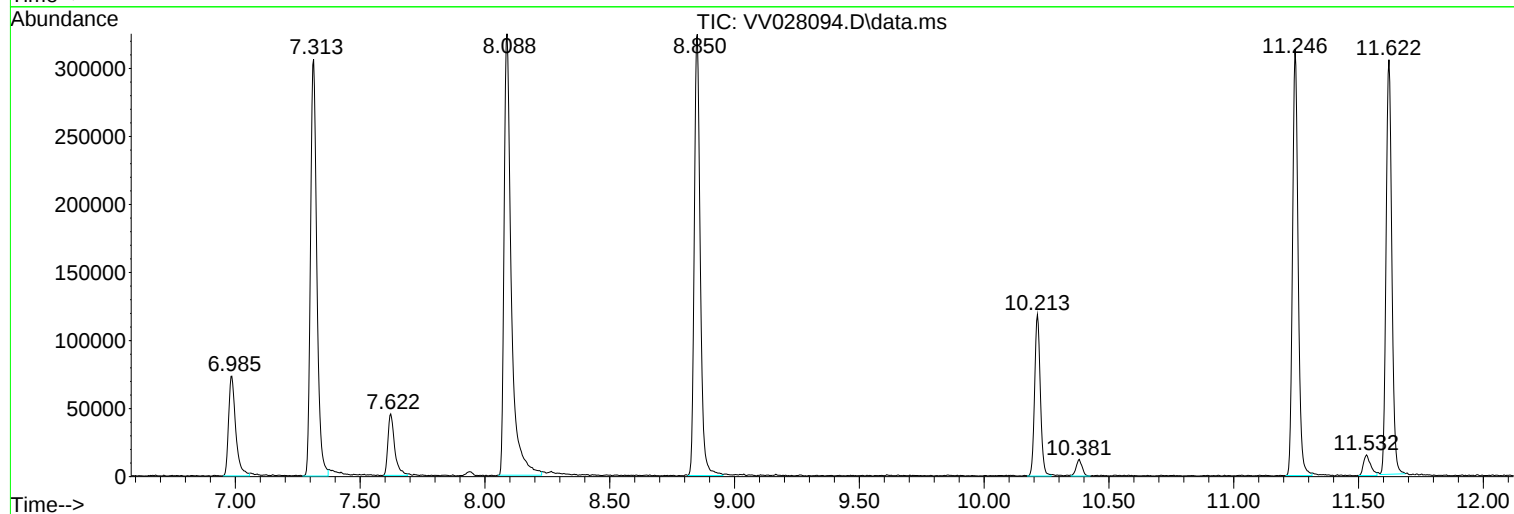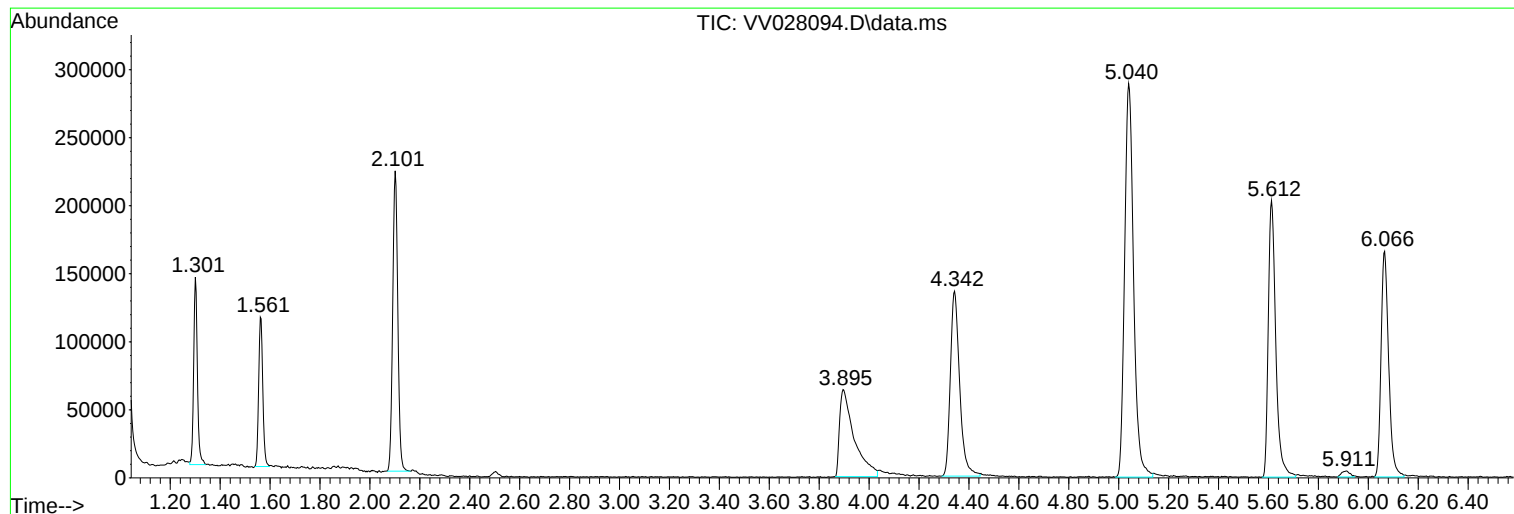

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028094.D
Acq On : 23 Sep 2022 11:24
Operator : SY/MD
Sample : N4729-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028094.D
Acq On : 23 Sep 2022 11:24
Operator : SY/MD
Sample : N4729-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc