

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028099.D
 Acq On : 23 Sep 2022 13:25
 Operator : SY/MD
 Sample : N4652-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	98	rVB	128830	136014	18.94%	2.283%
2	1.564	155	163	173	rBV	104719	121808	16.96%	2.044%
3	2.101	319	330	351	rVB	208370	296651	41.30%	4.979%
4	2.503	444	455	467	rBV3	12015	20063	2.79%	0.337%
5	3.899	877	889	935	rBV	63444	277803	38.68%	4.662%
6	4.342	1010	1027	1058	rBV2	128554	324720	45.21%	5.450%
7	5.040	1225	1244	1272	rBV3	288817	718265	100.00%	12.055%
8	5.612	1407	1422	1442	rBV	212682	434470	60.49%	7.292%
9	6.066	1550	1563	1591	rBV	164757	348558	48.53%	5.850%
10	6.982	1836	1848	1872	rBV	73981	146175	20.35%	2.453%
11	7.313	1938	1951	1974	rBV	308157	541394	75.38%	9.086%
12	7.622	2036	2047	2070	rBV	46605	87070	12.12%	1.461%
13	7.937	2133	2145	2156	rBV2	18990	34578	4.81%	0.580%
14	8.088	2179	2192	2227	rBV	331091	660283	91.93%	11.082%
15	8.850	2417	2429	2453	rBV	330279	550430	76.63%	9.238%
16	10.213	2840	2853	2870	rBV	120831	193647	26.96%	3.250%
17	10.381	2893	2905	2917	rBV	29925	49456	6.89%	0.830%
18	11.246	3163	3174	3195	rBV	326837	510502	71.07%	8.568%
19	11.622	3279	3291	3314	rBV	301417	488712	68.04%	8.202%
20	12.249	3474	3486	3495	rBV2	10623	17649	2.46%	0.296%




Sum of corrected areas: 5958248

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028099.D
Acq On : 23 Sep 2022 13:25
Operator : SY/MD
Sample : N4652-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

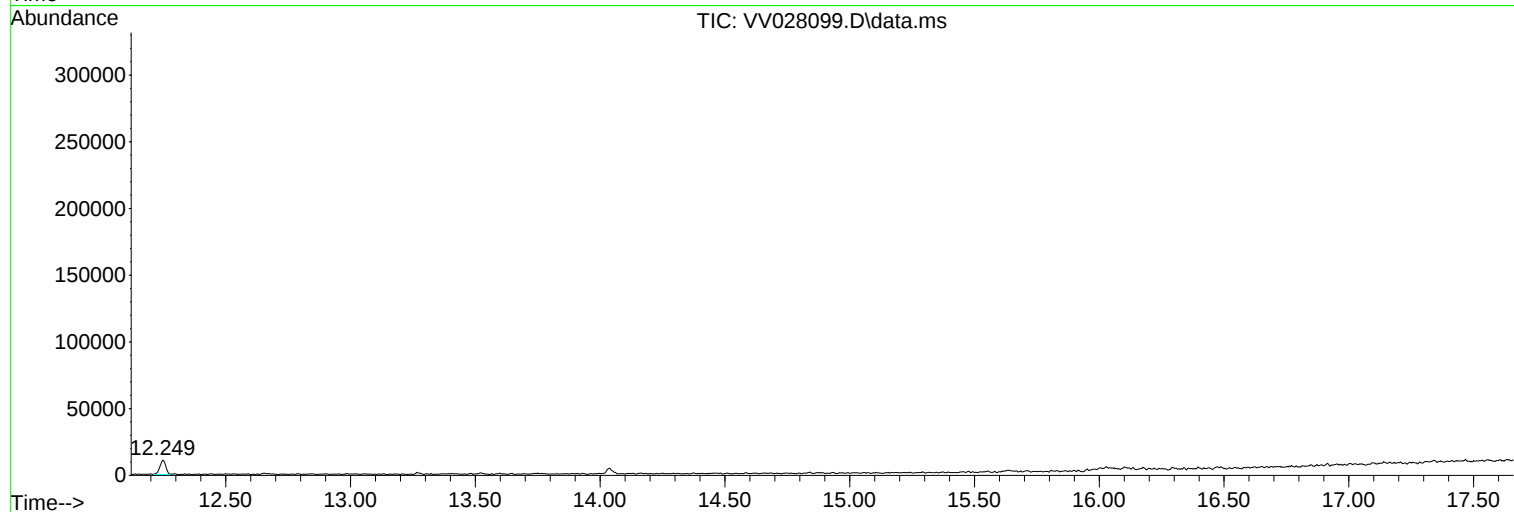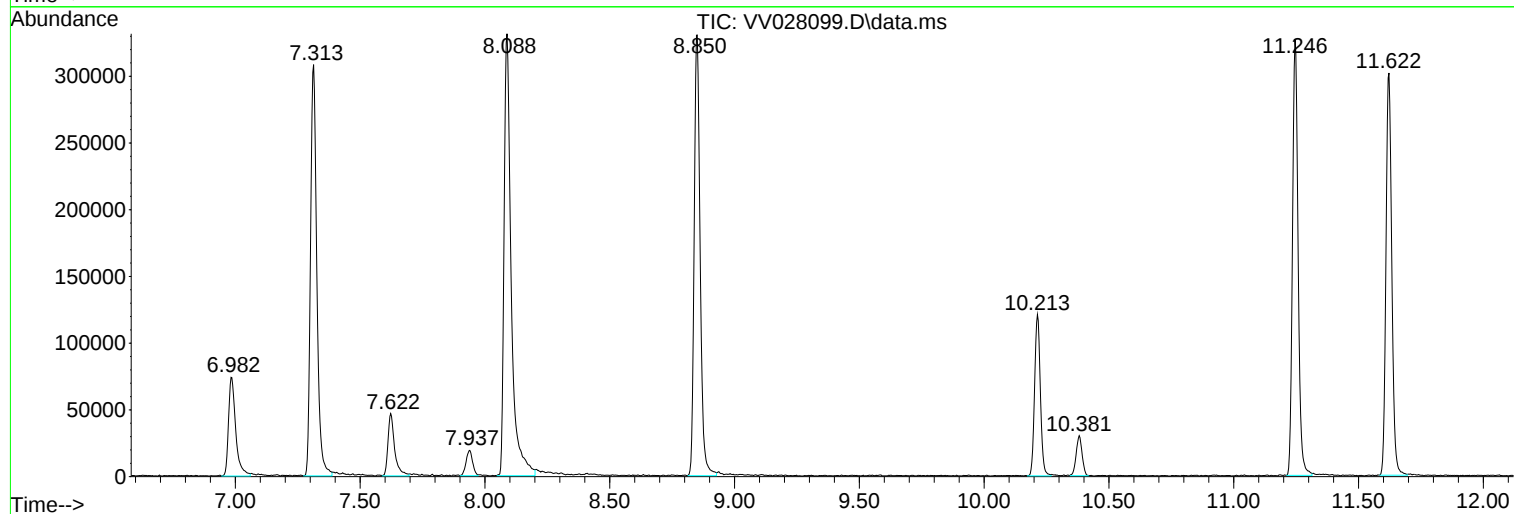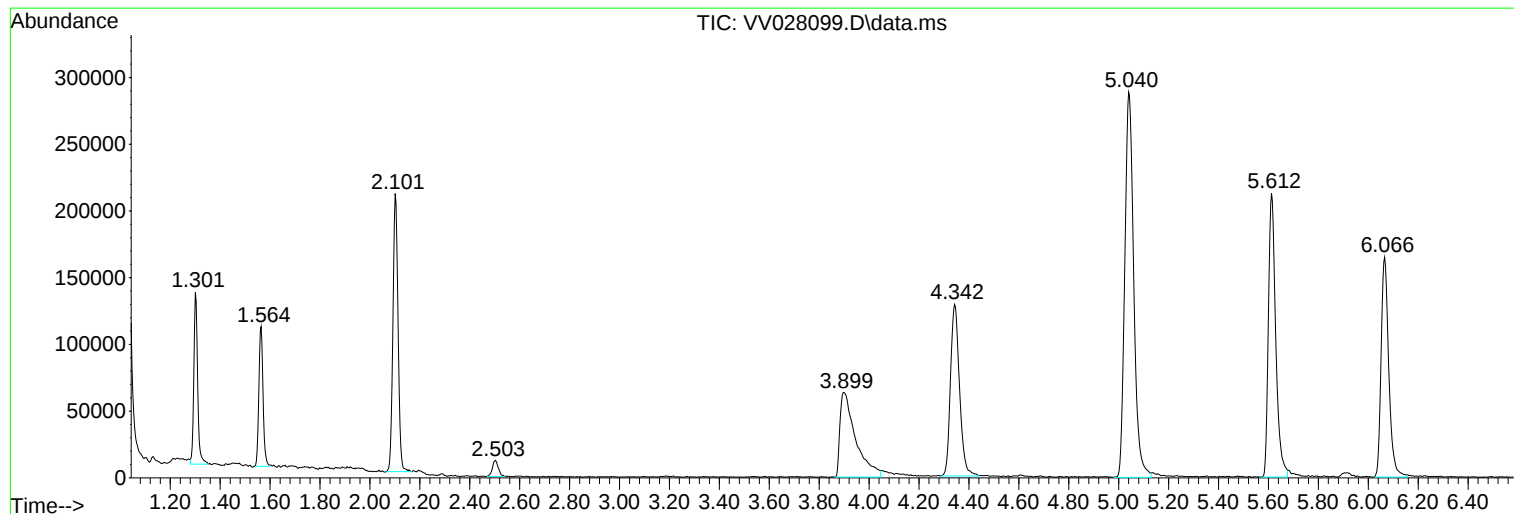

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028099.D
Acq On : 23 Sep 2022 13:25
Operator : SY/MD
Sample : N4652-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028099.D
Acq On : 23 Sep 2022 13:25
Operator : SY/MD
Sample : N4652-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc