

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028100.D
 Acq On : 23 Sep 2022 13:49
 Operator : SY/MD
 Sample : N4621-13 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8J8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	25	28	39	rVB2	9862	11477	1.58%	0.181%
2	1.301	74	81	97	rVB	133341	141133	19.41%	2.229%
3	1.561	155	162	175	rVB	108547	122373	16.83%	1.933%
4	2.101	319	330	342	rBV	213609	303426	41.73%	4.792%
5	2.500	446	454	463	rBV3	7538	12529	1.72%	0.198%
6	3.285	687	698	715	rBV3	6480	15336	2.11%	0.242%
7	3.908	880	892	932	rBV2	57026	292882	40.28%	4.626%
8	4.342	1008	1027	1050	rBV2	128876	330699	45.48%	5.223%
9	5.040	1227	1244	1269	rBV2	289462	727060	100.00%	11.483%
10	5.613	1410	1422	1447	rBV	197110	409793	56.36%	6.472%
11	6.066	1550	1563	1589	rBV2	167514	353740	48.65%	5.587%
12	6.985	1837	1849	1869	rBV	75473	145977	20.08%	2.305%
13	7.313	1939	1951	1968	rBV	307658	545437	75.02%	8.614%
14	7.622	2035	2047	2070	rBV	45917	88768	12.21%	1.402%
15	7.937	2133	2145	2156	rBV3	7555	14206	1.95%	0.224%
16	8.088	2182	2192	2225	rBV	345882	711605	97.87%	11.239%
17	8.850	2418	2429	2434	rBV	325817	541103	74.42%	8.546%
18	9.931	2754	2765	2774	rBV2	11183	16735	2.30%	0.264%
19	10.214	2842	2853	2867	rBV	132765	209189	28.77%	3.304%
20	10.381	2893	2905	2917	rVB	15523	29893	4.11%	0.472%
21	11.246	3163	3174	3199	rVV	316782	518392	71.30%	8.187%
22	11.448	3230	3237	3244	rBV7	4865	7370	1.01%	0.116%
23	11.525	3251	3261	3279	rVB	75817	133930	18.42%	2.115%
24	11.622	3279	3291	3307	rBV	333937	542823	74.66%	8.573%
25	12.017	3406	3414	3421	rBV3	8303	11718	1.61%	0.185%
26	12.114	3433	3444	3453	rBV	12030	18885	2.60%	0.298%
27	12.249	3479	3486	3494	rVB4	4922	7739	1.06%	0.122%
28	12.413	3525	3537	3548	rVB2	19919	30727	4.23%	0.485%
29	12.876	3668	3681	3689	rBV8	6205	10375	1.43%	0.164%
30	14.821	4275	4286	4295	rBV6	5811	9713	1.34%	0.153%
31	16.480	4793	4802	4813	rBV5	9626	16706	2.30%	0.264%




Sum of corrected areas: 6331739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028100.D
Acq On : 23 Sep 2022 13:49
Operator : SY/MD
Sample : N4621-13 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

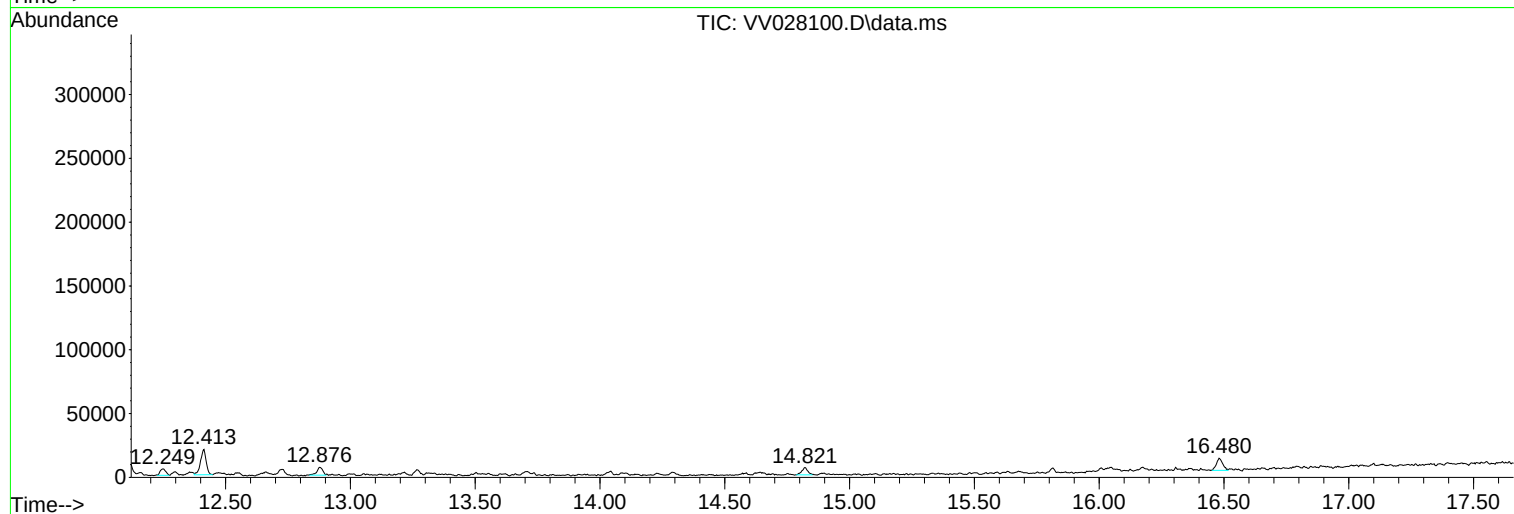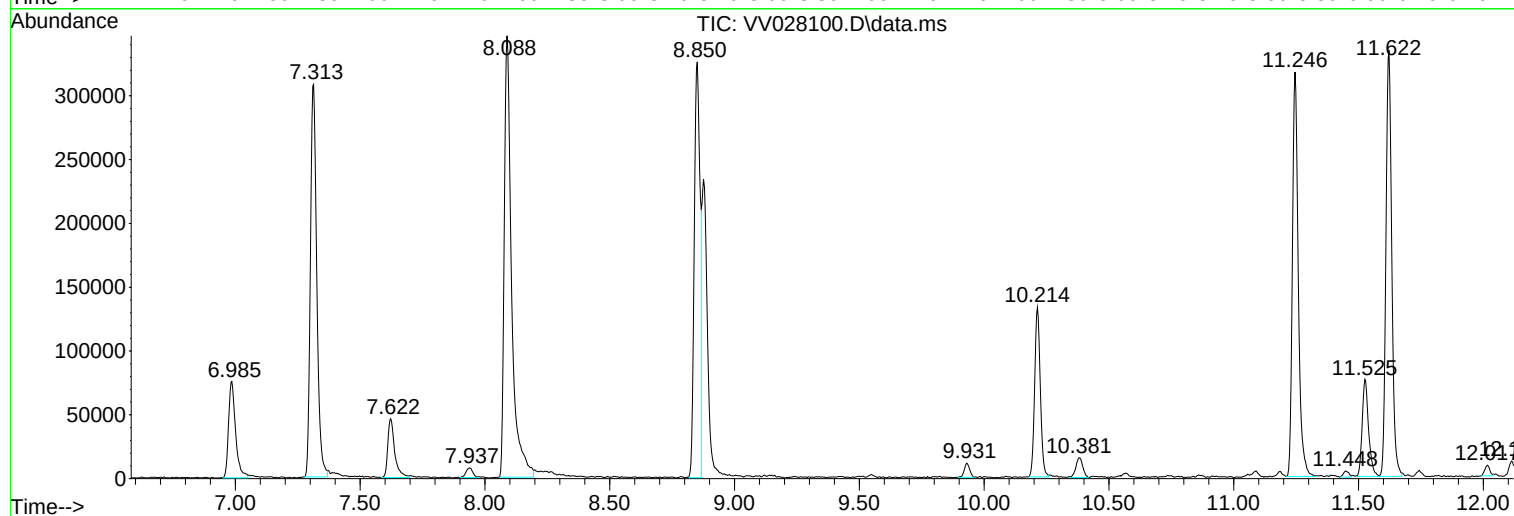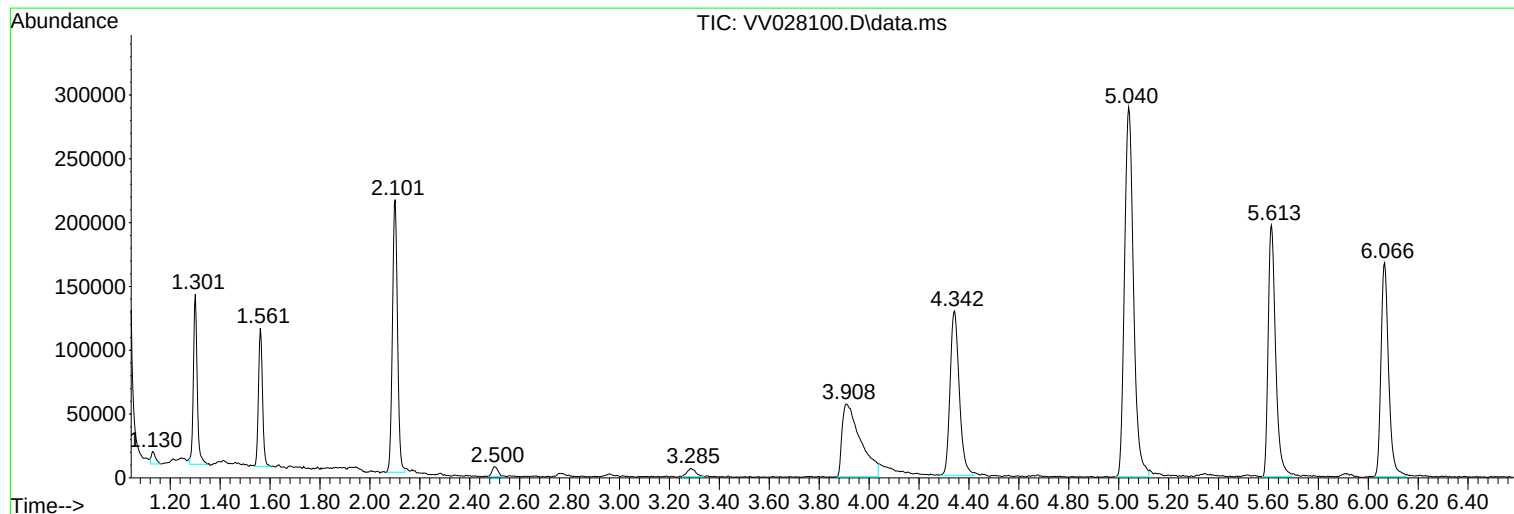

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028100.D
Acq On : 23 Sep 2022 13:49
Operator : SY/MD
Sample : N4621-13 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8J8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.525	1.29 ug/L	133930	1,4-Dichlorobenzene-d4	11.246

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane			118	C9H10	000496-11-7	94
2	Indane			118	C9H10	000496-11-7	94
3	Indane			118	C9H10	000496-11-7	81
4	7-Methylenecycloocta-1,3,5-triene			118	C9H10	002570-13-0	64
5	Tetracyclo[3.3.1.0(2,8).0(4,6)]-...			118	C9H10	1000191-13-7	64

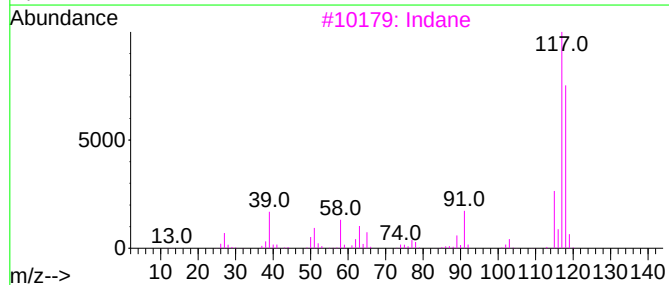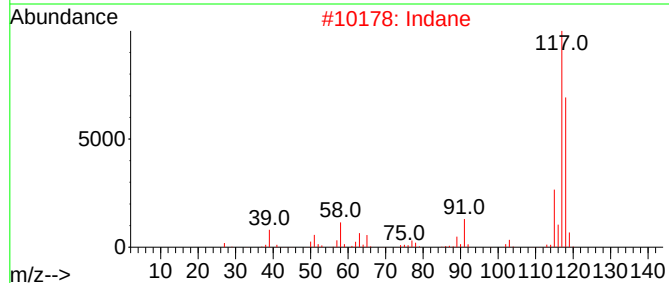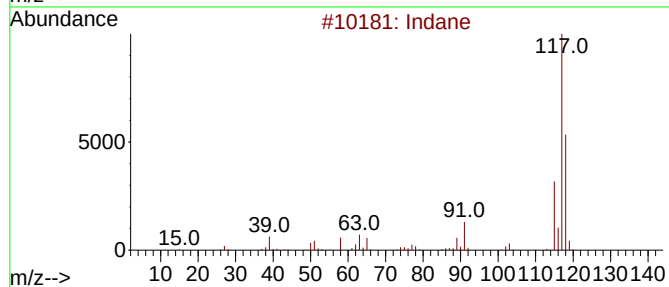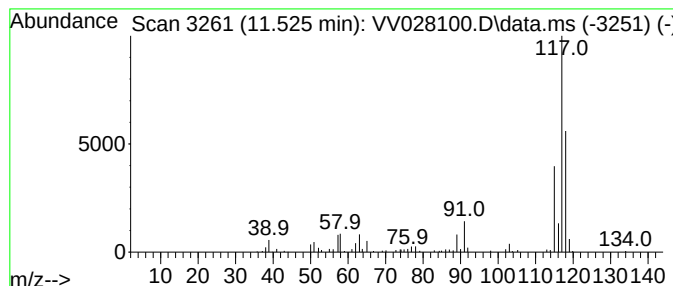

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028100.D
Acq On : 23 Sep 2022 13:49
Operator : SY/MD
Sample : N4621-13 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	11.525	1.3	ug/L	133930	3	11.246	518392	5.0