

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028102.D
 Acq On : 23 Sep 2022 14:38
 Operator : SY/MD
 Sample : N4621-15 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8K3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	24	28	39	rVB	11579	12763	1.74%	0.202%
2	1.301	74	81	95	rVB	122791	130936	17.90%	2.075%
3	1.561	155	162	174	rVB	102856	117914	16.12%	1.869%
4	2.098	319	329	341	rBV	206314	290502	39.72%	4.603%
5	2.500	443	454	466	rBV	12433	21715	2.97%	0.344%
6	2.767	527	537	548	rBV7	4090	8423	1.15%	0.133%
7	3.285	686	698	716	rBV3	7787	20722	2.83%	0.328%
8	3.912	880	893	933	rBV	50441	265906	36.35%	4.214%
9	4.339	1010	1026	1054	rBV2	131161	335402	45.85%	5.315%
10	5.040	1225	1244	1267	rBV2	296062	731441	100.00%	11.591%
11	5.613	1411	1422	1446	rBV	193034	401623	54.91%	6.364%
12	6.066	1548	1563	1591	rBV	171540	369847	50.56%	5.861%
13	6.986	1836	1849	1869	rBV	75533	145910	19.95%	2.312%
14	7.314	1938	1951	1971	rBV	299919	540247	73.86%	8.561%
15	7.622	2037	2047	2064	rBV	47853	89823	12.28%	1.423%
16	8.088	2180	2192	2223	rBV	338305	693197	94.77%	10.985%
17	8.850	2417	2429	2435	rBV	321790	556377	76.07%	8.817%
18	9.931	2757	2765	2775	rBV2	14713	23116	3.16%	0.366%
19	10.214	2834	2853	2867	rBV	128683	211435	28.91%	3.350%
20	10.387	2893	2907	2915	rBV5	5987	11538	1.58%	0.183%
21	11.246	3163	3174	3195	rVV	308364	495617	67.76%	7.854%
22	11.526	3250	3261	3280	rBV2	135616	217206	29.70%	3.442%
23	11.622	3280	3291	3312	rVB	330379	525891	71.90%	8.333%
24	12.014	3403	3413	3426	rBV5	8459	16583	2.27%	0.263%
25	12.114	3436	3444	3454	rVB4	10809	17206	2.35%	0.273%
26	12.410	3530	3536	3546	rVB2	9040	12185	1.67%	0.193%
27	12.718	3625	3632	3642	rVB3	7509	11144	1.52%	0.177%
28	12.882	3673	3683	3691	rVB6	12569	18922	2.59%	0.300%
29	16.480	4795	4802	4811	rBV3	9900	17009	2.33%	0.270%




Sum of corrected areas: 6310600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028102.D
Acq On : 23 Sep 2022 14:38
Operator : SY/MD
Sample : N4621-15 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

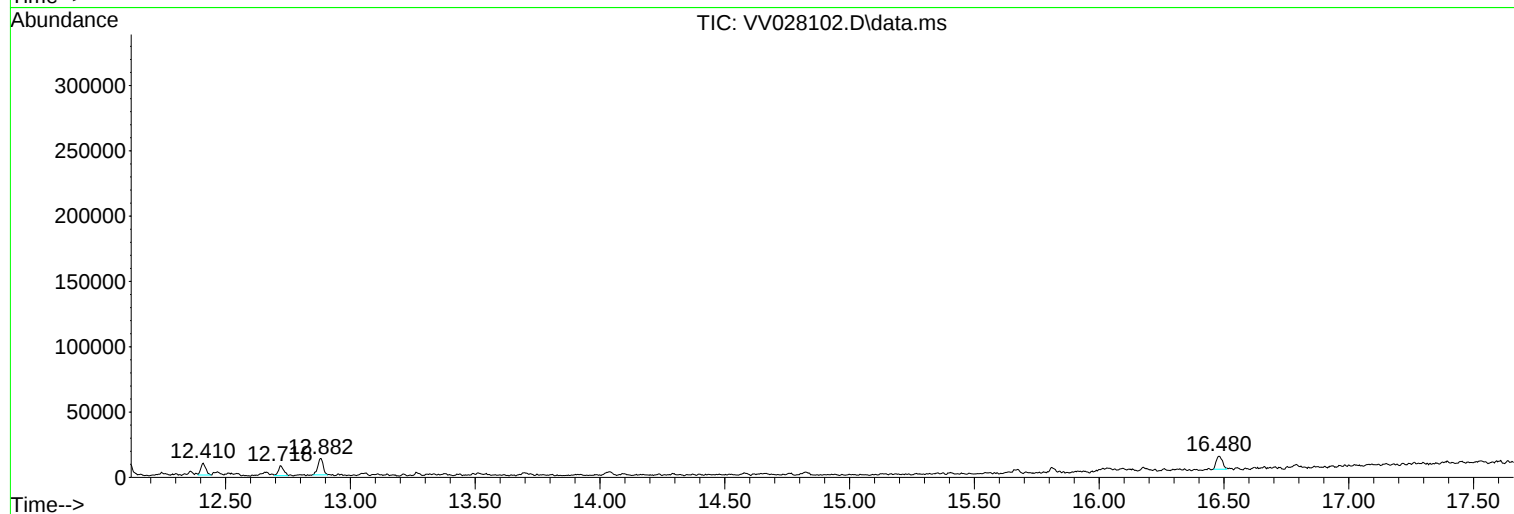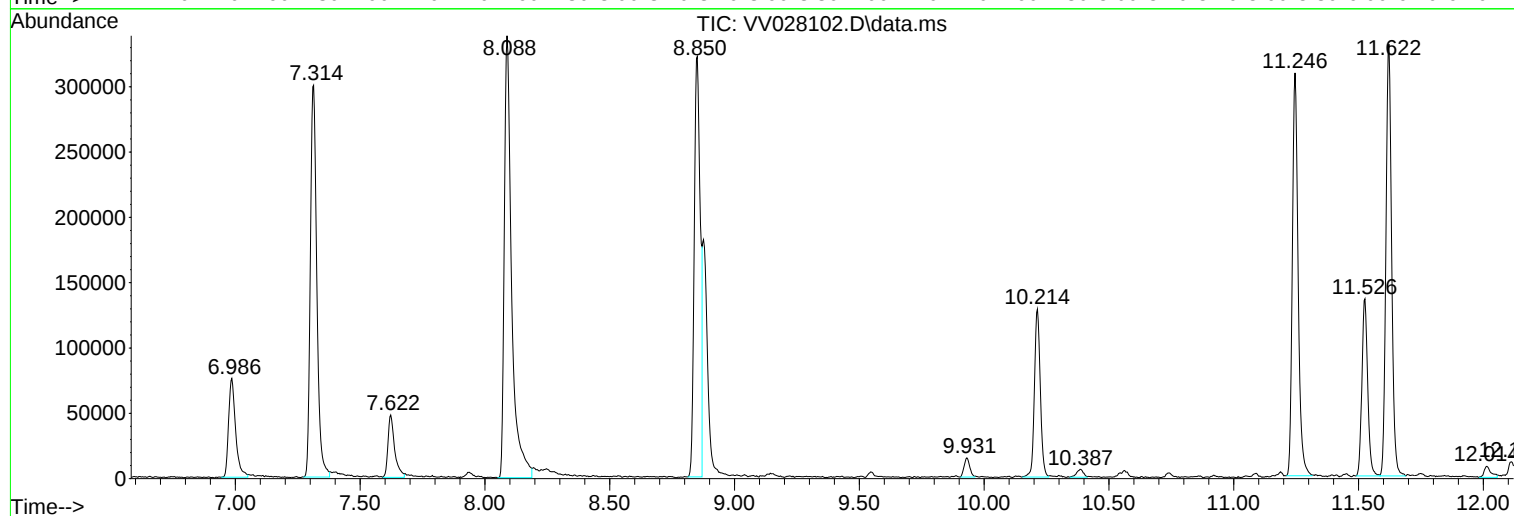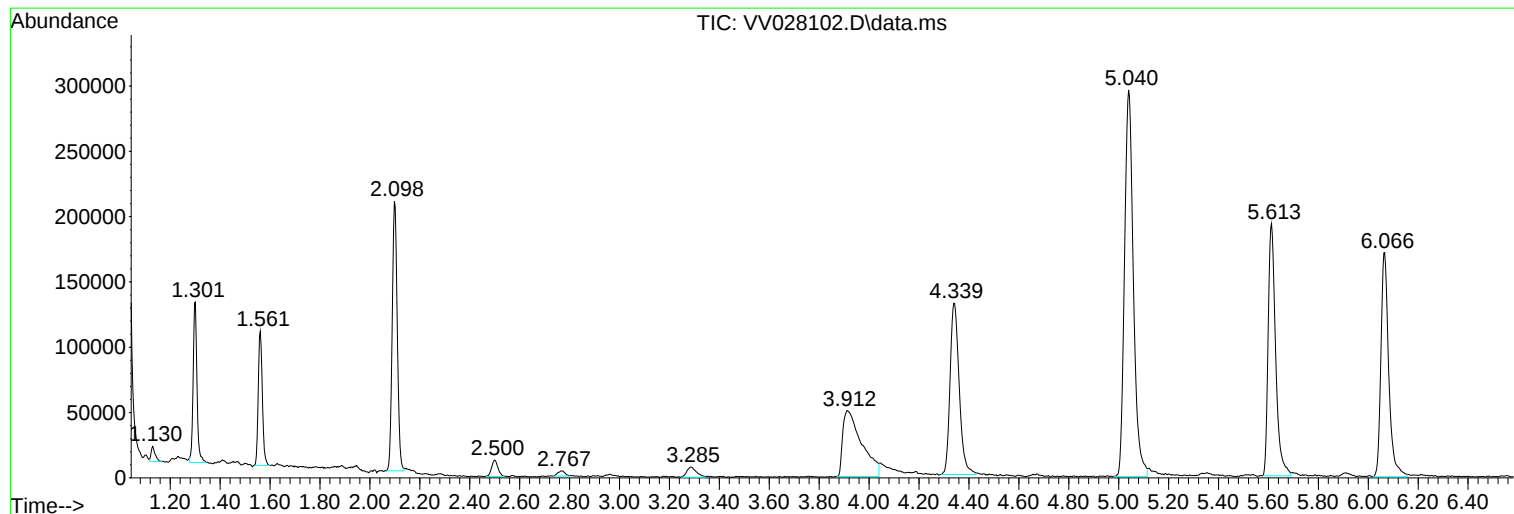

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028102.D
Acq On : 23 Sep 2022 14:38
Operator : SY/MD
Sample : N4621-15 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028102.D
Acq On : 23 Sep 2022 14:38
Operator : SY/MD
Sample : N4621-15 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc