

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028106.D
 Acq On : 23 Sep 2022 16:15
 Operator : SY/MD
 Sample : VIBLK293
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK293

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	116894	124653	17.69%	2.121%
2	1.561	155	162	177	rVB	101245	116904	16.59%	1.989%
3	2.101	320	330	344	rVB	187957	269596	38.26%	4.588%
4	2.503	445	455	466	rBV2	13762	22693	3.22%	0.386%
5	3.880	870	883	915	rBV2	95486	283527	40.24%	4.825%
6	4.343	1006	1027	1050	rBV	131748	332052	47.12%	5.651%
7	5.040	1228	1244	1266	rBV2	282013	704622	100.00%	11.991%
8	5.613	1408	1422	1449	rBV	190724	405802	57.59%	6.906%
9	5.912	1503	1515	1536	rBV	85248	180133	25.56%	3.065%
10	6.066	1550	1563	1586	rBV2	169553	355083	50.39%	6.042%
11	6.986	1836	1849	1867	rBV2	75185	144193	20.46%	2.454%
12	7.313	1938	1951	1977	rBV	292038	525656	74.60%	8.945%
13	7.622	2036	2047	2066	rBV2	44137	83994	11.92%	1.429%
14	7.934	2137	2144	2156	rVB3	5915	10117	1.44%	0.172%
15	8.085	2177	2191	2232	rBV	349947	687851	97.62%	11.705%
16	8.850	2415	2429	2454	rBV	303653	512462	72.73%	8.721%
17	10.214	2842	2853	2868	rBV	124874	198299	28.14%	3.374%
18	10.378	2894	2904	2915	rVB	9662	15963	2.27%	0.272%
19	11.246	3164	3174	3192	rBV	280706	443505	62.94%	7.547%
20	11.622	3279	3291	3315	rBV	284327	459340	65.19%	7.817%




Sum of corrected areas: 5876445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028106.D
Acq On : 23 Sep 2022 16:15
Operator : SY/MD
Sample : VIBLK293
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

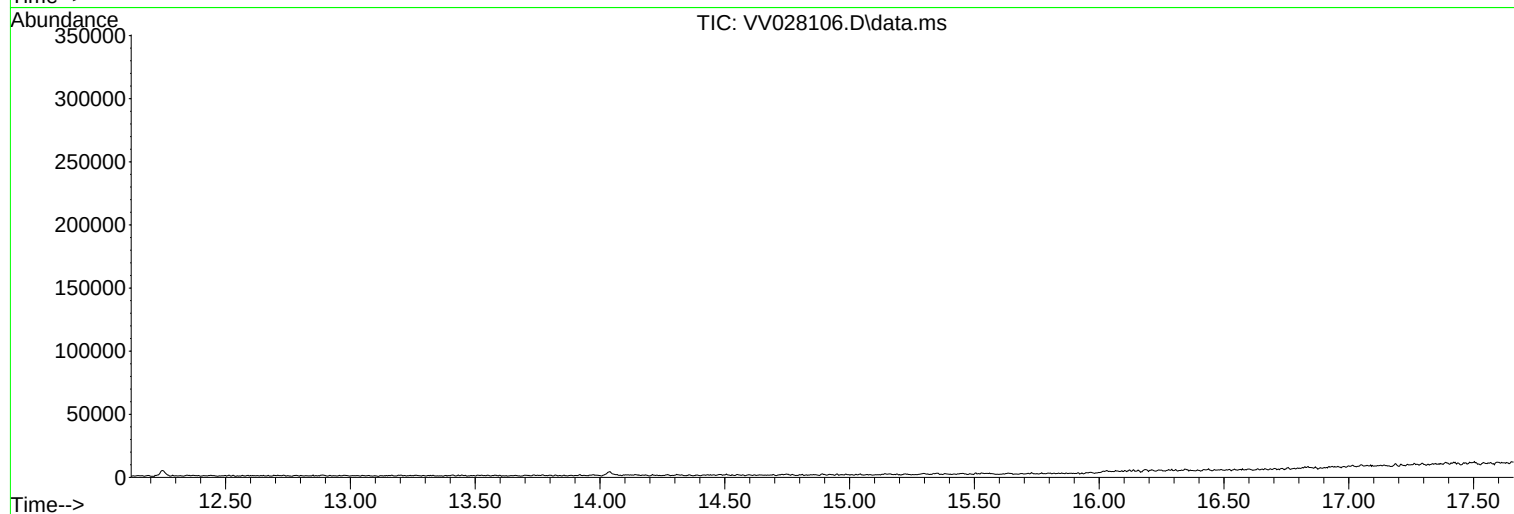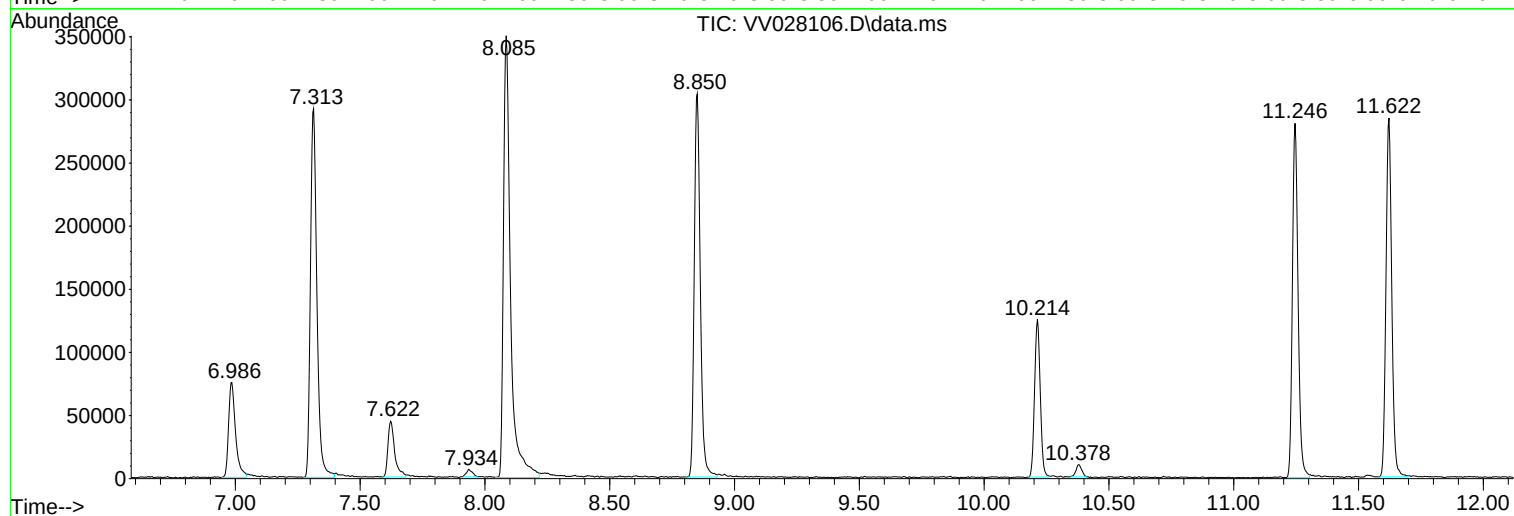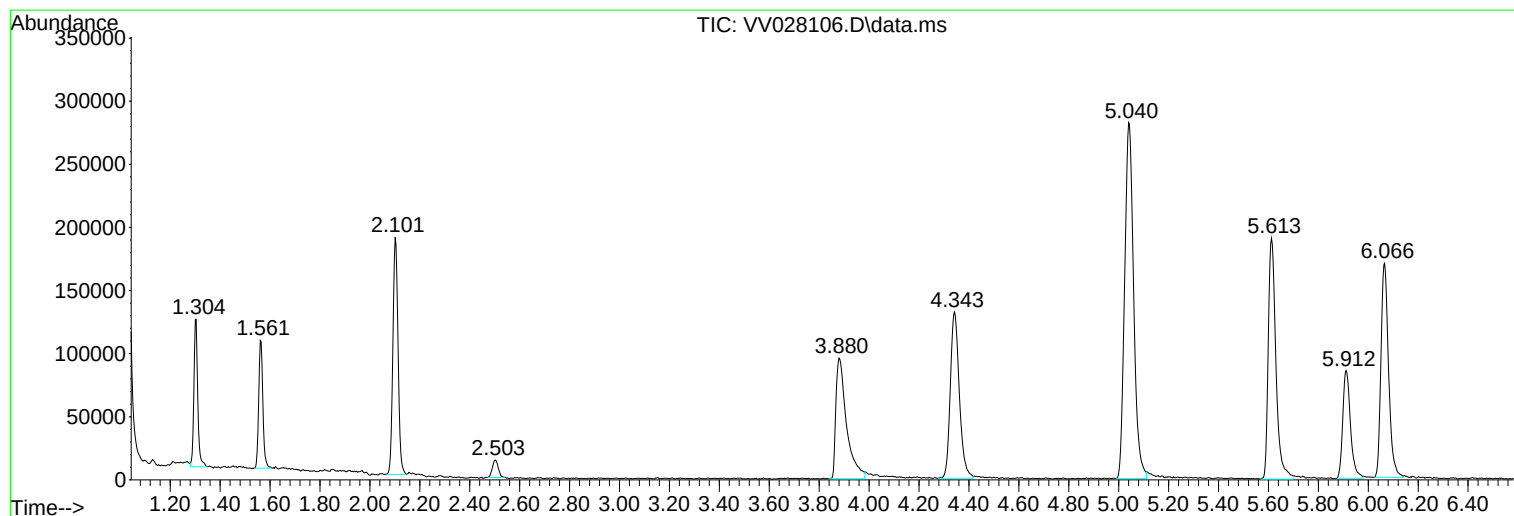

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028106.D
Acq On : 23 Sep 2022 16:15
Operator : SY/MD
Sample : VIBLK293
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028106.D
Acq On : 23 Sep 2022 16:15
Operator : SY/MD
Sample : VIBLK293
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------