

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
 Data File : VV028107.D
 Acq On : 23 Sep 2022 17:22
 Operator : SY/MD
 Sample : VIBLK294
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK294

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	25	28	37	rVB2	5375	6835	1.01%	0.124%
2	1.301	74	81	96	rVB	114255	121279	17.85%	2.201%
3	1.561	155	162	172	rBV	98470	110263	16.23%	2.001%
4	2.098	319	329	342	rBV	184151	258058	37.98%	4.684%
5	2.500	442	454	467	rBV	19974	35833	5.27%	0.650%
6	3.902	878	890	920	rBV	56439	236723	34.84%	4.296%
7	4.336	1009	1025	1054	rBV	126026	319162	46.98%	5.793%
8	5.037	1228	1243	1273	rBV2	270174	679403	100.00%	12.331%
9	5.609	1406	1421	1452	rBV	195505	411366	60.55%	7.466%
10	5.915	1504	1516	1533	rBV4	20123	47929	7.05%	0.870%
11	6.063	1549	1562	1587	rBV	161104	341413	50.25%	6.196%
12	6.982	1835	1848	1870	rBV	71070	139058	20.47%	2.524%
13	7.310	1938	1950	1974	rBV	271436	495034	72.86%	8.985%
14	7.622	2038	2047	2072	rBV2	41381	77646	11.43%	1.409%
15	8.085	2181	2191	2229	rBV	315567	652349	96.02%	11.840%
16	8.847	2417	2428	2453	rBV	304611	515227	75.84%	9.351%
17	10.214	2841	2853	2873	rVB	120684	193032	28.41%	3.503%
18	11.246	3163	3174	3190	rBV	279968	444019	65.35%	8.059%
19	11.622	3279	3291	3305	rBV	266206	425203	62.58%	7.717%




Sum of corrected areas: 5509832

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028107.D
Acq On : 23 Sep 2022 17:22
Operator : SY/MD
Sample : VIBLK294
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

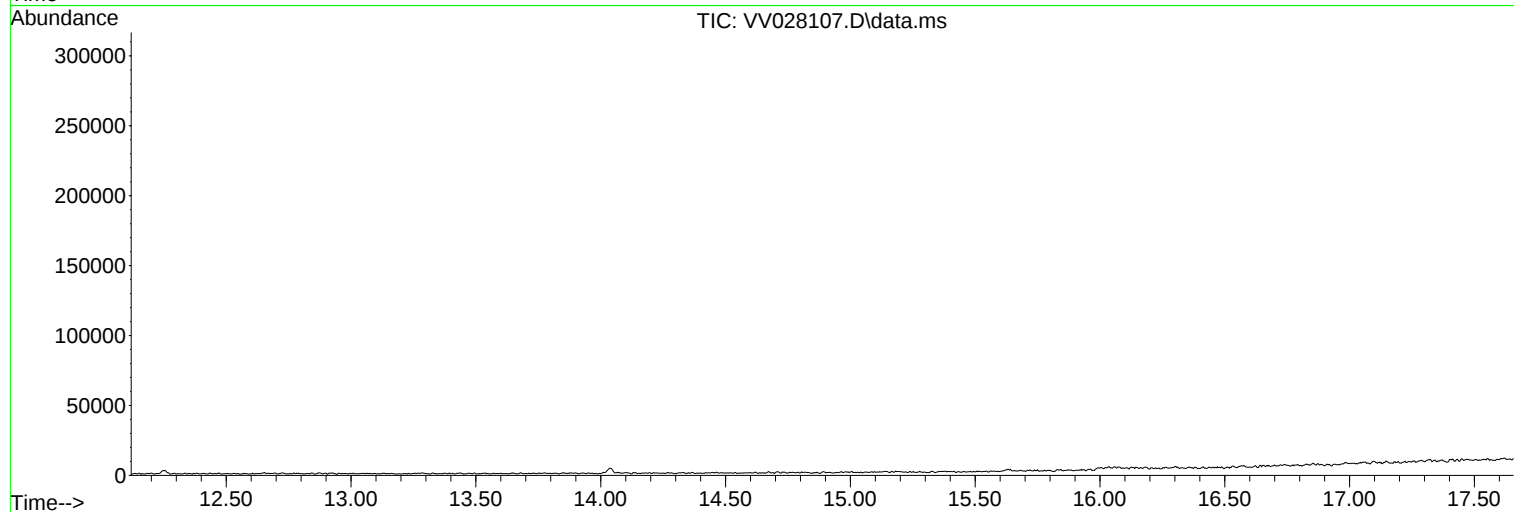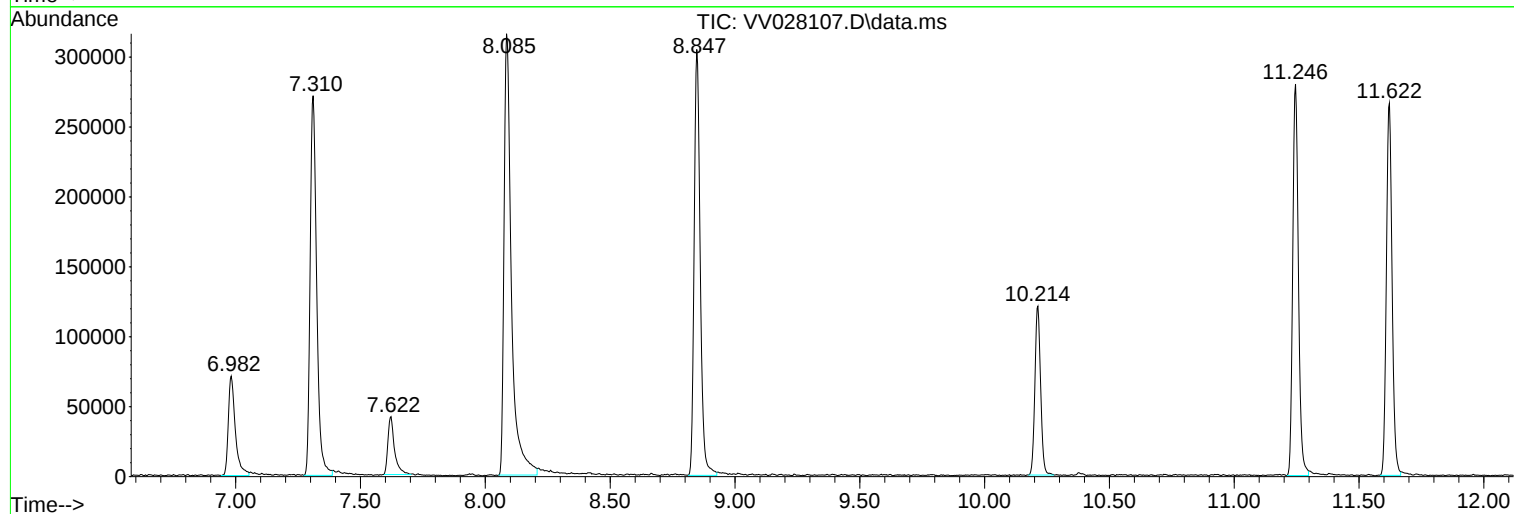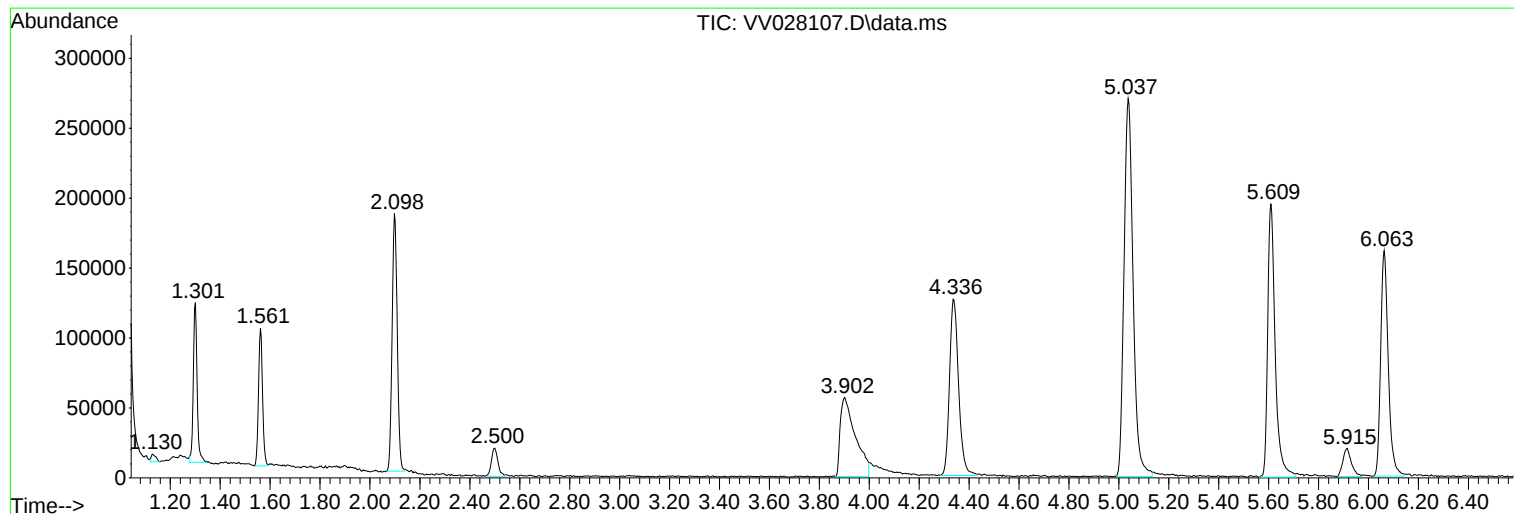

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028107.D
Acq On : 23 Sep 2022 17:22
Operator : SY/MD
Sample : VIBLK294
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028107.D
Acq On : 23 Sep 2022 17:22
Operator : SY/MD
Sample : VIBLK294
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc