
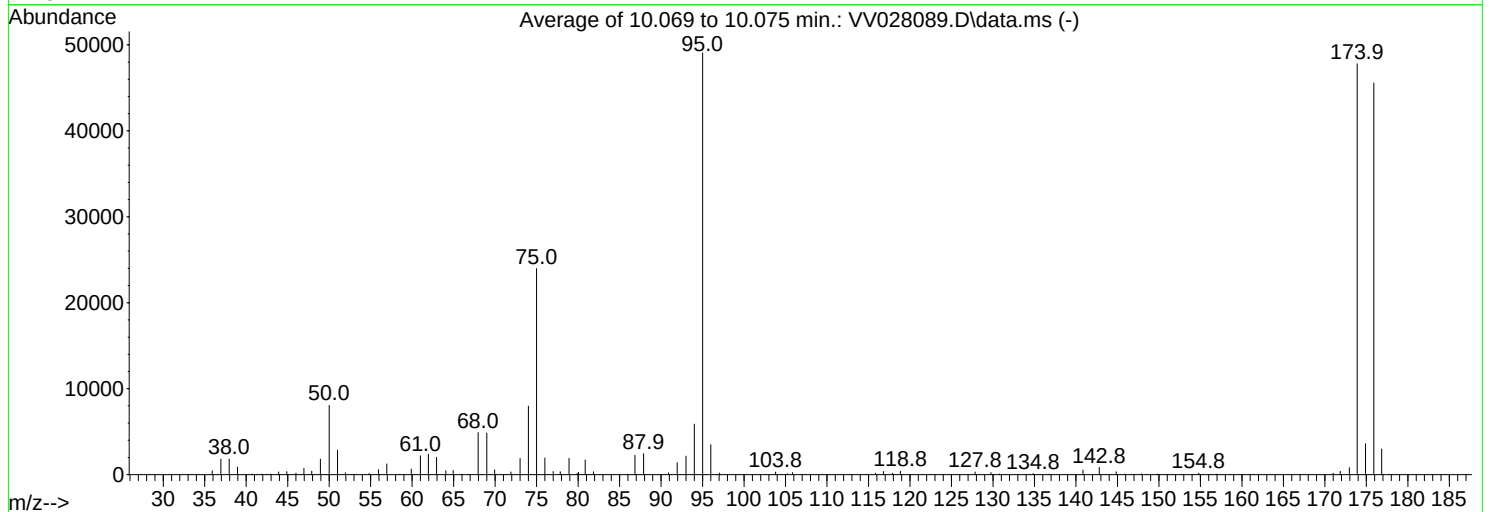


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092322\
Data File : VV028089.D
Acq On : 23 Sep 2022 09:03
Operator : SY/MD
Sample : BFB375
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB375

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Sep 26 21:28:54 2022

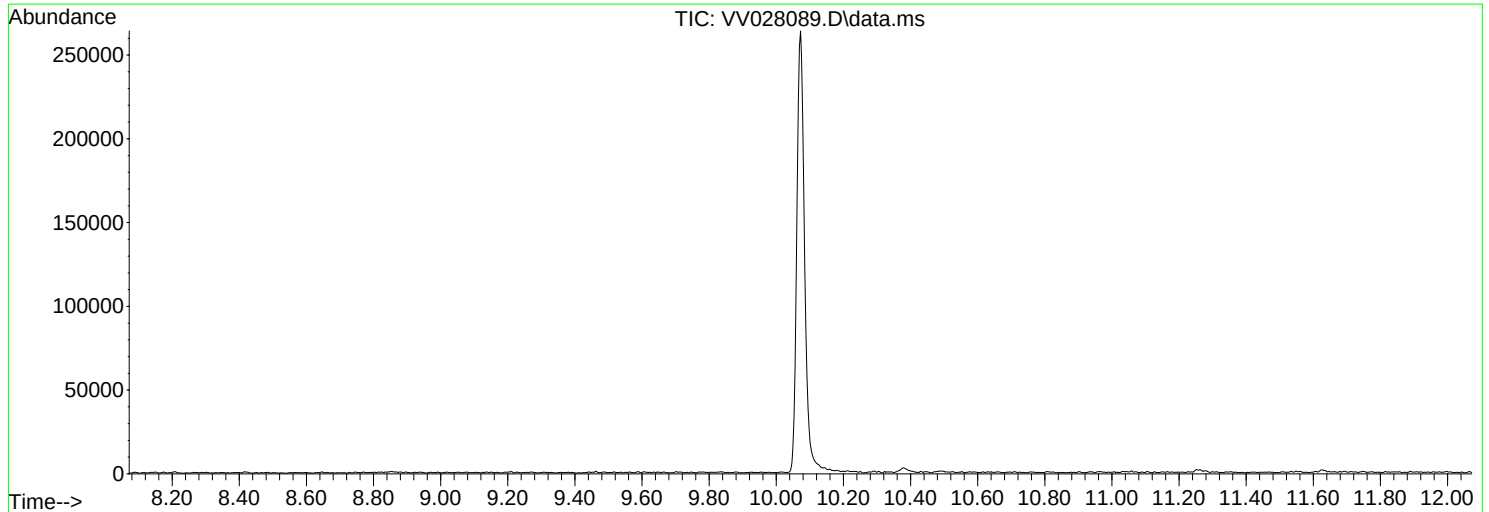

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	8063	PASS
75	95	30	80	48.9	23979	PASS
95	95	100	100	100.0	49077	PASS
96	95	5	9	7.1	3487	PASS
173	174	0.00	2	1.7	808	PASS
174	95	50	120	97.4	47800	PASS
175	174	5	9	7.5	3594	PASS
176	174	95	105	95.3	45573	PASS
177	176	5	10	6.5	2975	PASS

m/z	Abundance
39.90	267.0
41.20	103.0
43.90	389.0
45.10	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

m/z	Abundance
35.90	483.0
37.00	1801.0
38.00	1835.0
38.90	778.0
40.10	298.0
41.10	112.0
42.90	113.0
43.90	668.0
44.90	456.0
46.00	165.0
46.90	728.0
47.90	405.0
48.90	1840.0
50.00	8173.0
51.00	2703.0
52.00	196.0
54.90	141.0
55.90	630.0
57.00	1173.0
58.50	103.0
59.90	638.0
61.00	2264.0
62.00	2333.0
63.00	1991.0
64.10	549.0
65.00	487.0
66.80	120.0
68.00	4976.0
69.00	4875.0
70.00	521.0
71.90	288.0
73.00	1911.0
74.00	8145.0
75.00	24232.0
76.00	2110.0
77.00	371.0
77.80	281.0
78.90	2002.0
79.90	447.0
80.90	1667.0
82.00	301.0
86.90	2352.0
87.90	2531.0
90.90	201.0
92.00	1418.0
93.00	2159.0
94.00	5921.0
95.00	49024.0
96.00	3497.0
97.00	197.0
102.70	106.0
103.80	295.0
105.20	129.0
105.90	269.0
115.80	167.0
116.80	390.0
117.80	179.0
118.80	403.0
127.90	271.0
129.70	200.0
130.80	104.0
134.80	130.0
136.80	158.0
140.90	507.0
142.80	851.0
144.80	309.0
149.80	124.0
152.80	133.0
154.80	154.0
156.90	116.0
171.00	164.0
171.90	400.0
172.90	771.0
173.90	46928.0
174.90	3450.0
175.90	44816.0
176.80	3092.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

m/z	Abundance
35.90	467.0
37.00	1817.0
37.90	1883.0
38.90	900.0
40.00	272.0
40.70	116.0
41.90	120.0
42.90	119.0
44.00	734.0
44.90	528.0
46.00	194.0
47.00	735.0
47.90	433.0
49.00	1847.0
50.00	8175.0
51.00	2963.0
51.90	243.0
54.80	145.0
55.90	603.0
57.00	1310.0
59.90	673.0
61.00	2249.0
62.00	2399.0
62.90	2083.0
64.00	469.0
64.90	500.0
68.00	5093.0
69.00	5071.0
69.90	598.0
71.90	334.0
73.00	1953.0
74.00	8265.0
75.00	24904.0
76.00	1956.0
77.00	390.0
77.90	360.0
78.90	1954.0
80.10	454.0
80.80	1735.0
81.80	337.0
86.90	2332.0
87.90	2472.0
90.90	217.0
91.90	1450.0
93.00	2216.0
94.00	6053.0
95.00	50504.0
96.00	3637.0
97.10	201.0
103.80	316.0
105.20	132.0
105.80	268.0
115.80	167.0
116.80	396.0
117.90	164.0
118.90	397.0
127.90	252.0
129.70	245.0
130.80	103.0
134.80	129.0
140.80	551.0
142.80	836.0
144.90	365.0
145.90	121.0
147.90	115.0
149.80	120.0
154.80	172.0
156.90	110.0
158.60	103.0
171.00	157.0
171.90	397.0
173.00	856.0
173.90	49408.0
174.90	3724.0
175.90	47096.0
176.80	3055.0
177.70	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

m/z	Abundance
35.90	403.0
36.90	1775.0
37.90	1725.0
39.00	970.0
39.90	253.0
40.70	122.0
41.30	103.0
41.90	116.0
42.50	105.0
44.00	712.0
44.90	452.0
46.00	213.0
47.00	690.0
47.90	377.0
49.00	1741.0
50.00	7840.0
51.00	2891.0
51.90	252.0
54.70	127.0
56.00	517.0
56.90	1253.0
59.90	630.0
61.00	2066.0
61.90	2342.0
62.90	1998.0
64.00	387.0
64.90	463.0
66.00	131.0
67.90	4640.0
69.00	4565.0
69.90	577.0
71.30	104.0
71.90	327.0
73.00	1801.0
74.00	7518.0
75.00	22800.0
76.00	1745.0
77.00	348.0
77.90	342.0
78.90	1755.0
80.00	413.0
80.80	1766.0
81.70	363.0
85.90	144.0
86.80	2059.0
87.90	2342.0
90.90	202.0
91.90	1315.0
93.00	2110.0
94.00	5667.0
95.00	47704.0
96.00	3328.0
97.10	194.0
103.80	309.0
105.20	103.0
105.80	205.0
112.70	121.0
114.70	119.0
115.90	163.0
116.80	338.0
118.00	151.0
118.90	392.0
127.70	214.0
127.90	219.0
129.80	268.0
134.90	112.0
140.80	550.0
142.80	812.0
144.90	347.0
145.90	124.0
147.90	159.0
154.80	162.0
171.00	190.0
171.80	359.0
172.90	797.0
173.90	47064.0
174.90	3607.0
175.90	44808.0
176.90	2779.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375