

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092722\
 Data File : VV028130.D
 Acq On : 27 Sep 2022 11:16
 Operator : SY/MD
 Sample : VV0927WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK236

Quant Time: Sep 28 03:08:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 28 03:08:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	170028	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	172409	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	78380	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	73421	4.165	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.400%
7) Chloroethane-d5	1.561	69	66449	4.741	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.800%
11) 1,1-Dichloroethene-d2	2.098	63	98071	3.208	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.200%
20) 2-Butanone-d5	3.902	46	178071	59.837	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.680%
24) Chloroform-d	4.339	84	147435	5.241	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%
26) 1,2-Dichloroethane-d4	5.024	65	72246	5.398	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.000%
32) Benzene-d6	5.040	84	268711	4.753	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
36) 1,2-Dichloropropane-d6	6.063	67	89924	5.102	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.000%
41) Toluene-d8	7.310	98	208091	4.067	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	7.619	79	29462	4.628	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.600%
46) 2-Hexanone-d5	8.085	63	144332	54.322	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.640%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	65355	5.425	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.600%
66) 1,2-Dichlorobenzene-d4	11.619	152	86401	5.620	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.400%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	9192	0.701	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092722\
Data File : VV028130.D
Acq On : 27 Sep 2022 11:16
Operator : SY/MD
Sample : VV0927WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK236

Quant Time: Sep 28 03:08:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 28 03:08:11 2022
Response via : Initial Calibration

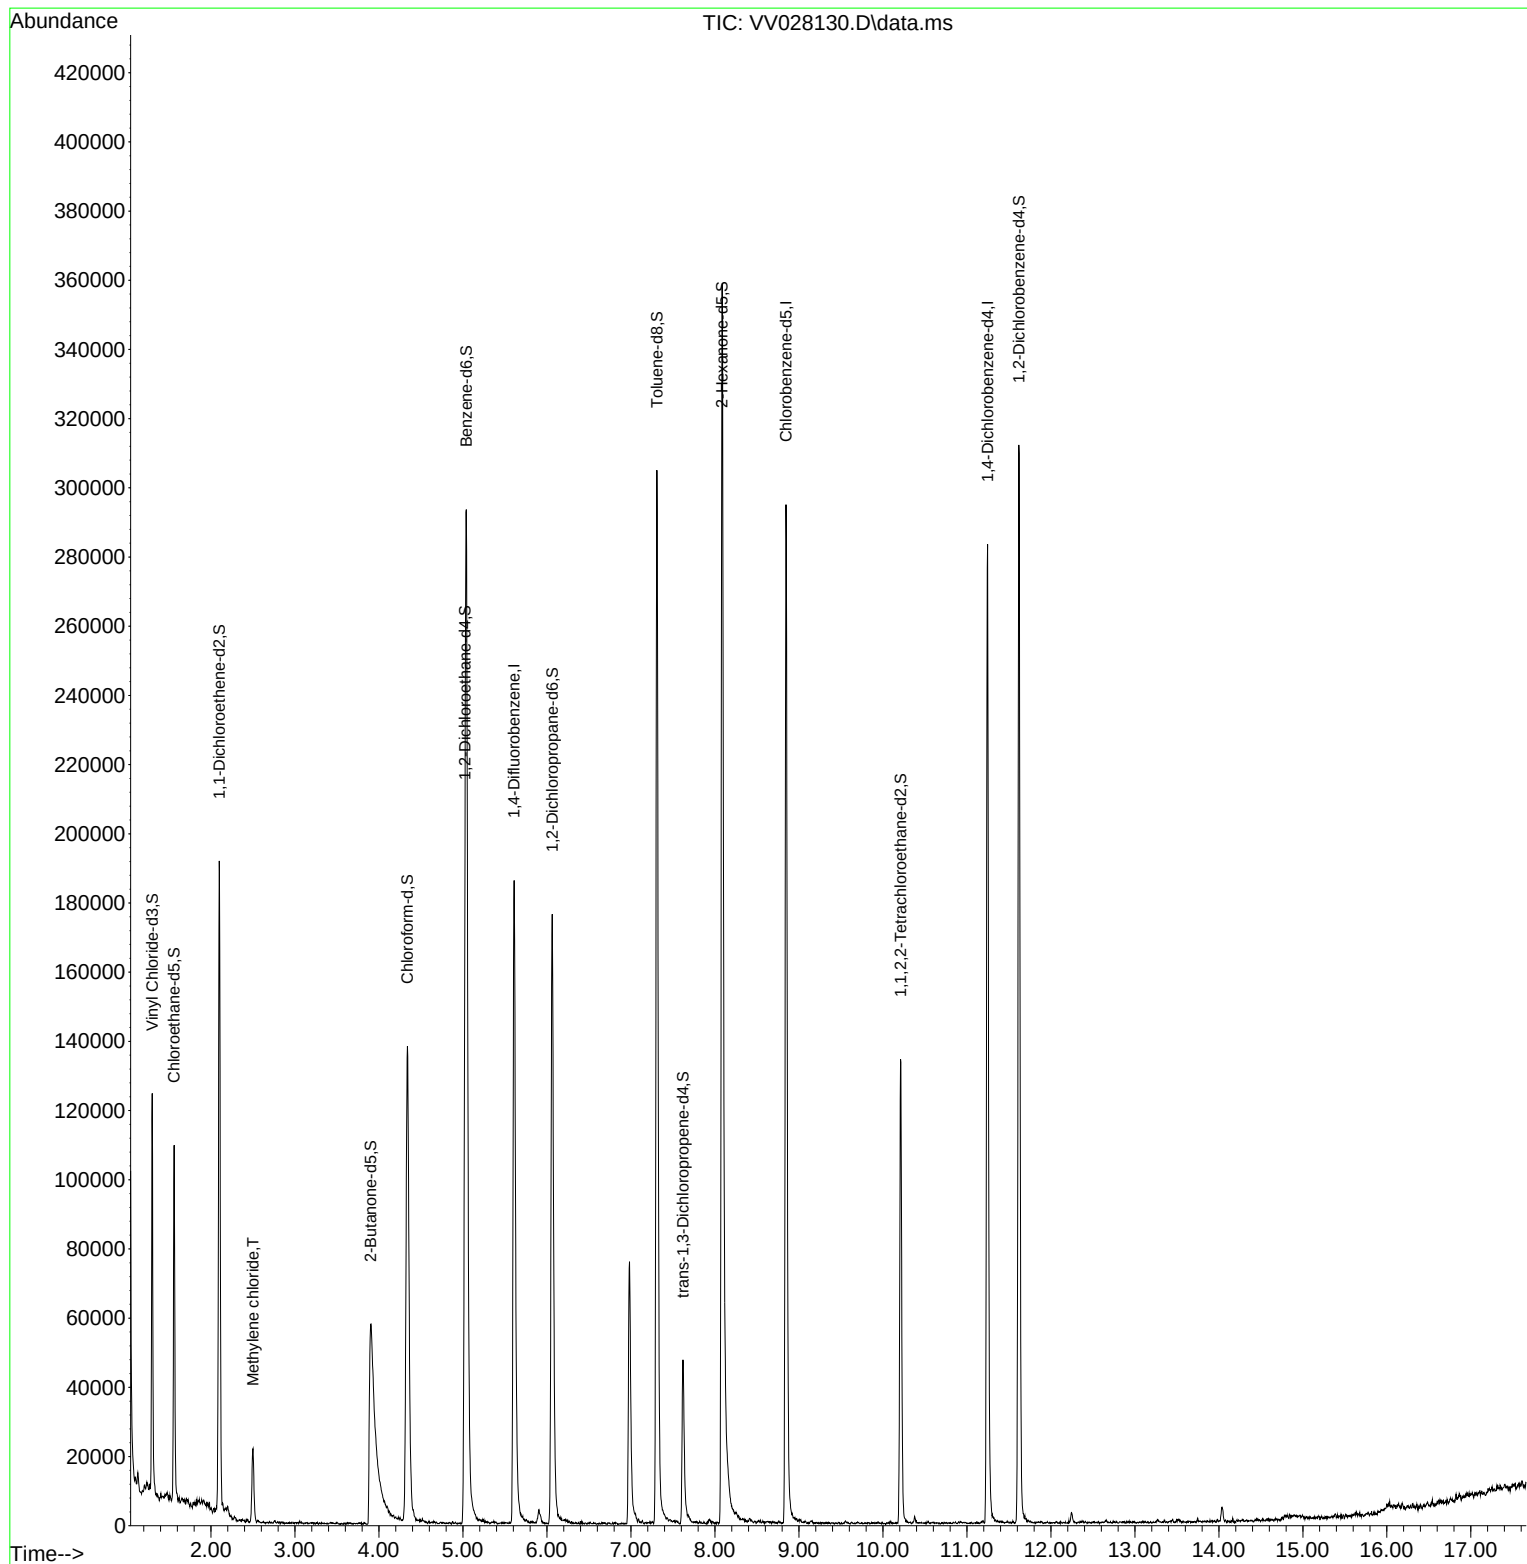

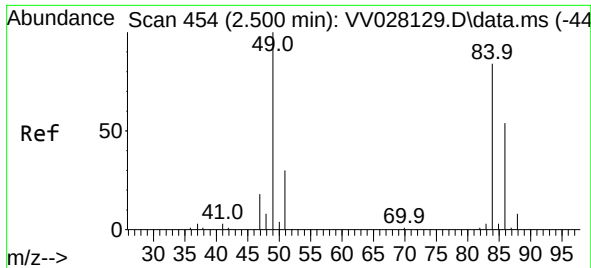

#16

Methylene chloride

Concen: 0.701 ug/L

RT: 2.500 min Scan# 4

Delta R.T. 0.000 min

Lab File: VV028130.D


Acq: 27 Sep 2022 11:16

Instrument :

MSVOA_V

ClientSampleId :

VBLK236

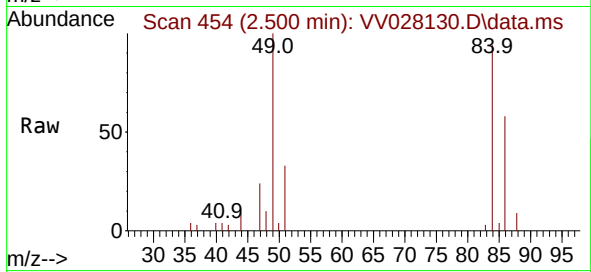

Tgt Ion: 84 Resp: 9192

Ion Ratio Lower Upper

84 100

86 62.1 46.8 86.8

49 106.8 87.5 162.5

