
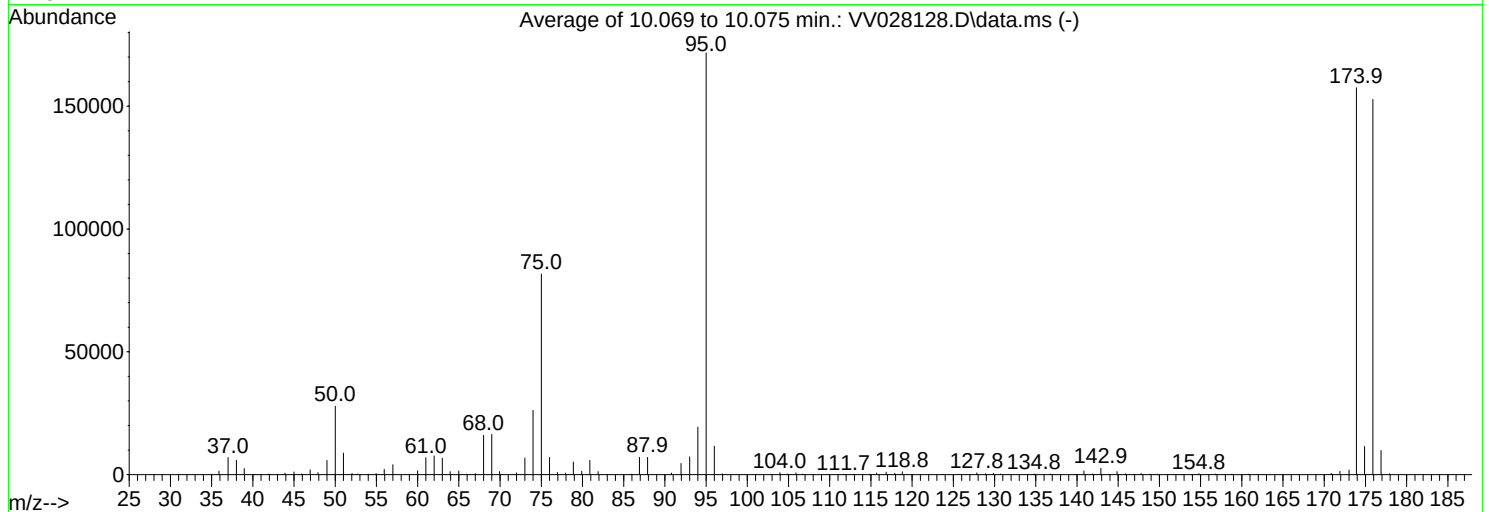


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092722\
Data File : VV028128.D
Acq On : 27 Sep 2022 09:10
Operator : SY/MD
Sample : BFB377
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB377

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 29 01:25:35 2022

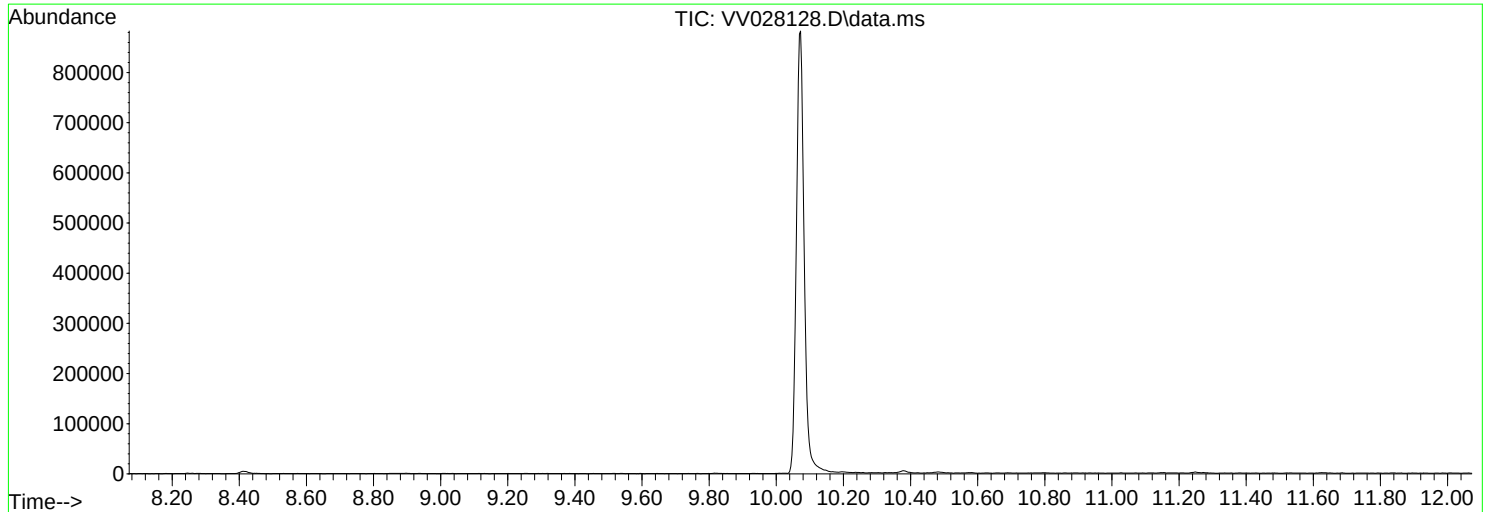

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	27851	PASS
75	95	30	80	47.6	81693	PASS
95	95	100	100	100.0	171712	PASS
96	95	5	9	6.7	11584	PASS
173	174	0.00	2	1.2	1920	PASS
174	95	50	120	91.7	157525	PASS
175	174	5	9	7.3	11453	PASS
176	174	95	105	97.0	152768	PASS
177	176	5	10	6.4	9837	PASS

m/z	Abundance
35.90	291.0
38.10	163.0
38.90	112.0
39.80	252.0
42.20	119.0
43.90	315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

m/z	Abundance
35.00	177.0
35.90	1721.0
37.00	7217.0
38.00	6422.0
39.00	2678.0
40.20	345.0
41.10	158.0
41.90	223.0
43.00	137.0
43.90	948.0
45.00	1230.0
45.90	288.0
47.00	2063.0
47.80	905.0
49.00	6179.0
50.00	28816.0
51.00	9421.0
52.10	467.0
52.80	284.0
54.00	228.0
55.00	449.0
55.90	2296.0
57.00	4198.0
58.00	148.0
60.00	1694.0
61.00	7242.0
62.00	8016.0
63.00	7063.0
64.00	1362.0
65.00	1567.0
66.00	215.0
67.00	478.0
68.00	16528.0
69.00	17512.0
70.00	1392.0
72.00	748.0
73.00	6866.0
74.00	26976.0
75.00	84448.0
76.00	7172.0
76.90	845.0
77.90	749.0
78.90	5416.0
79.90	1349.0
80.90	6025.0
81.90	1225.0
83.00	164.0
86.00	394.0
86.90	7535.0
87.90	7028.0
90.80	680.0
92.00	4937.0
93.00	7309.0
94.00	20008.0
95.00	176128.0
96.00	11882.0
97.00	333.0
102.90	173.0
103.90	741.0
104.80	275.0
105.90	708.0
106.80	271.0
109.80	115.0
111.00	105.0
111.70	138.0
112.90	140.0
114.90	265.0
115.70	655.0
116.90	1120.0
117.80	540.0
118.80	1303.0
123.90	134.0
127.80	667.0
128.90	347.0
129.90	651.0
130.80	219.0
134.80	290.0
136.90	276.0
139.70	123.0
140.90	1634.0
141.90	368.0
142.90	2765.0
143.90	148.0
144.80	1400.0
145.90	396.0
146.90	137.0
147.90	510.0
148.80	166.0
149.70	237.0
151.70	134.0
152.70	120.0
153.00	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

154.80	480.0
156.80	243.0
158.80	246.0
160.90	183.0
170.80	511.0
171.90	1265.0
173.00	1955.0
173.90	159168.0
174.90	11969.0
175.90	154112.0
176.90	10424.0
177.90	440.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

m/z	Abundance
35.00	166.0
35.90	1788.0
37.00	7224.0
38.00	6269.0
39.00	2629.0
41.00	144.0
41.90	206.0
42.90	134.0
43.90	954.0
45.00	1181.0
45.90	281.0
47.00	2003.0
47.90	884.0
49.00	5962.0
50.00	28752.0
51.00	9071.0
52.00	434.0
52.80	287.0
54.00	223.0
54.90	482.0
55.90	2204.0
57.00	4178.0
58.00	106.0
60.00	1634.0
61.00	7147.0
62.00	7931.0
63.00	6887.0
63.90	1213.0
65.00	1551.0
65.90	231.0
67.00	437.0
68.00	16600.0
69.00	16968.0
69.90	1300.0
72.00	757.0
73.00	7044.0
74.00	27032.0
75.00	84640.0
76.00	7267.0
77.00	919.0
78.00	698.0
78.90	5262.0
79.90	1382.0
80.90	5974.0
81.90	1234.0
83.00	153.0
85.90	294.0
86.90	7299.0
87.90	7352.0
90.80	659.0
92.00	4706.0
93.00	7549.0
94.00	20000.0
95.00	177792.0
96.00	11994.0
96.90	322.0
102.80	166.0
104.00	784.0
104.80	271.0
105.90	755.0
106.70	224.0
109.80	113.0
111.70	127.0
112.90	174.0
114.90	216.0
115.70	666.0
116.90	1077.0
117.90	623.0
118.80	1232.0
123.70	128.0
125.60	118.0
127.00	122.0
127.90	773.0
128.90	336.0
129.90	619.0
130.70	251.0
134.80	272.0
136.70	265.0
139.70	110.0
140.90	1534.0
141.90	316.0
142.90	2681.0
143.90	169.0
144.90	1311.0
145.90	383.0
146.90	187.0
147.80	477.0
148.90	191.0
149.80	217.0
151.70	142.0
153.00	141.0
153.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

154.80	429.0
156.80	273.0
158.80	228.0
160.80	211.0
170.90	526.0
171.90	1410.0
173.00	1950.0
173.90	162368.0
174.90	11783.0
175.90	157952.0
176.90	10186.0
177.90	375.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

m/z	Abundance
36.00	1647.0
37.00	6438.0
38.00	5417.0
39.00	2372.0
39.80	288.0
40.90	118.0
41.90	125.0
42.90	122.0
43.90	879.0
45.00	1018.0
45.90	234.0
46.90	1771.0
48.00	836.0
49.00	5297.0
50.00	25984.0
51.00	7967.0
52.00	396.0
52.70	235.0
54.00	186.0
54.90	450.0
56.00	1932.0
57.00	3843.0
58.10	112.0
60.00	1380.0
61.00	6382.0
62.00	6976.0
63.00	6237.0
63.90	1055.0
65.00	1398.0
65.90	213.0
67.00	340.0
68.00	15025.0
69.00	14755.0
69.90	1097.0
72.00	720.0
73.00	6434.0
74.00	24616.0
75.00	75992.0
76.00	6563.0
77.00	939.0
78.00	603.0
78.90	4742.0
79.90	1380.0
80.90	5365.0
81.90	1210.0
82.90	128.0
85.70	250.0
86.90	6253.0
87.90	6762.0
90.80	543.0
91.90	4053.0
93.00	6942.0
94.00	18000.0
95.00	161216.0
96.00	10876.0
96.90	251.0
102.80	115.0
104.00	742.0
104.90	234.0
105.90	676.0
106.60	207.0
107.00	195.0
108.00	114.0
111.90	108.0
112.90	182.0
114.80	172.0
115.70	556.0
116.80	997.0
118.00	703.0
118.80	1038.0
123.70	108.0
125.60	118.0
127.10	130.0
127.90	759.0
128.90	289.0
129.80	535.0
130.70	274.0
134.80	234.0
136.70	273.0
140.80	1326.0
141.90	221.0
142.90	2305.0
143.80	160.0
144.90	1117.0
145.90	323.0
146.90	170.0
147.70	450.0
148.90	170.0
149.90	199.0
151.80	126.0
152.90	136.0
154.80	355.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

156.80	292.0
158.80	199.0
160.80	219.0
170.90	511.0
171.90	1374.0
173.00	1854.0
173.90	151040.0
174.90	10606.0
175.90	146240.0
176.90	8900.0
177.90	239.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377