

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
 Data File : VV028242.D
 Acq On : 30 Sep 2022 22:06
 Operator : SY/MD
 Sample : VV0930WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Quant Time: Oct 01 02:17:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	165465	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	167241	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	75923	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	70018	4.082	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.600%
7) Chloroethane-d5	1.561	69	61876	4.537	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.800%
11) 1,1-Dichloroethene-d2	2.098	63	102938	3.460	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.200%
20) 2-Butanone-d5	3.899	46	129937	44.867	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.740%
24) Chloroform-d	4.339	84	128711	4.702	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
26) 1,2-Dichloroethane-d4	5.027	65	62964	4.834	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
32) Benzene-d6	5.043	84	269363	4.912	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
36) 1,2-Dichloropropane-d6	6.063	67	79062	4.625	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.400%
41) Toluene-d8	7.310	98	220805	4.449	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%
43) trans-1,3-Dichloroprop...	7.622	79	25244	4.088	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.800%
46) 2-Hexanone-d5	8.088	63	115025	44.629	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.260%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	56479	4.833	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	79804	5.359	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.200%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.500	84	8122	0.636	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028242.D
Acq On : 30 Sep 2022 22:06
Operator : SY/MD
Sample : VV0930WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Time: Oct 01 02:17:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

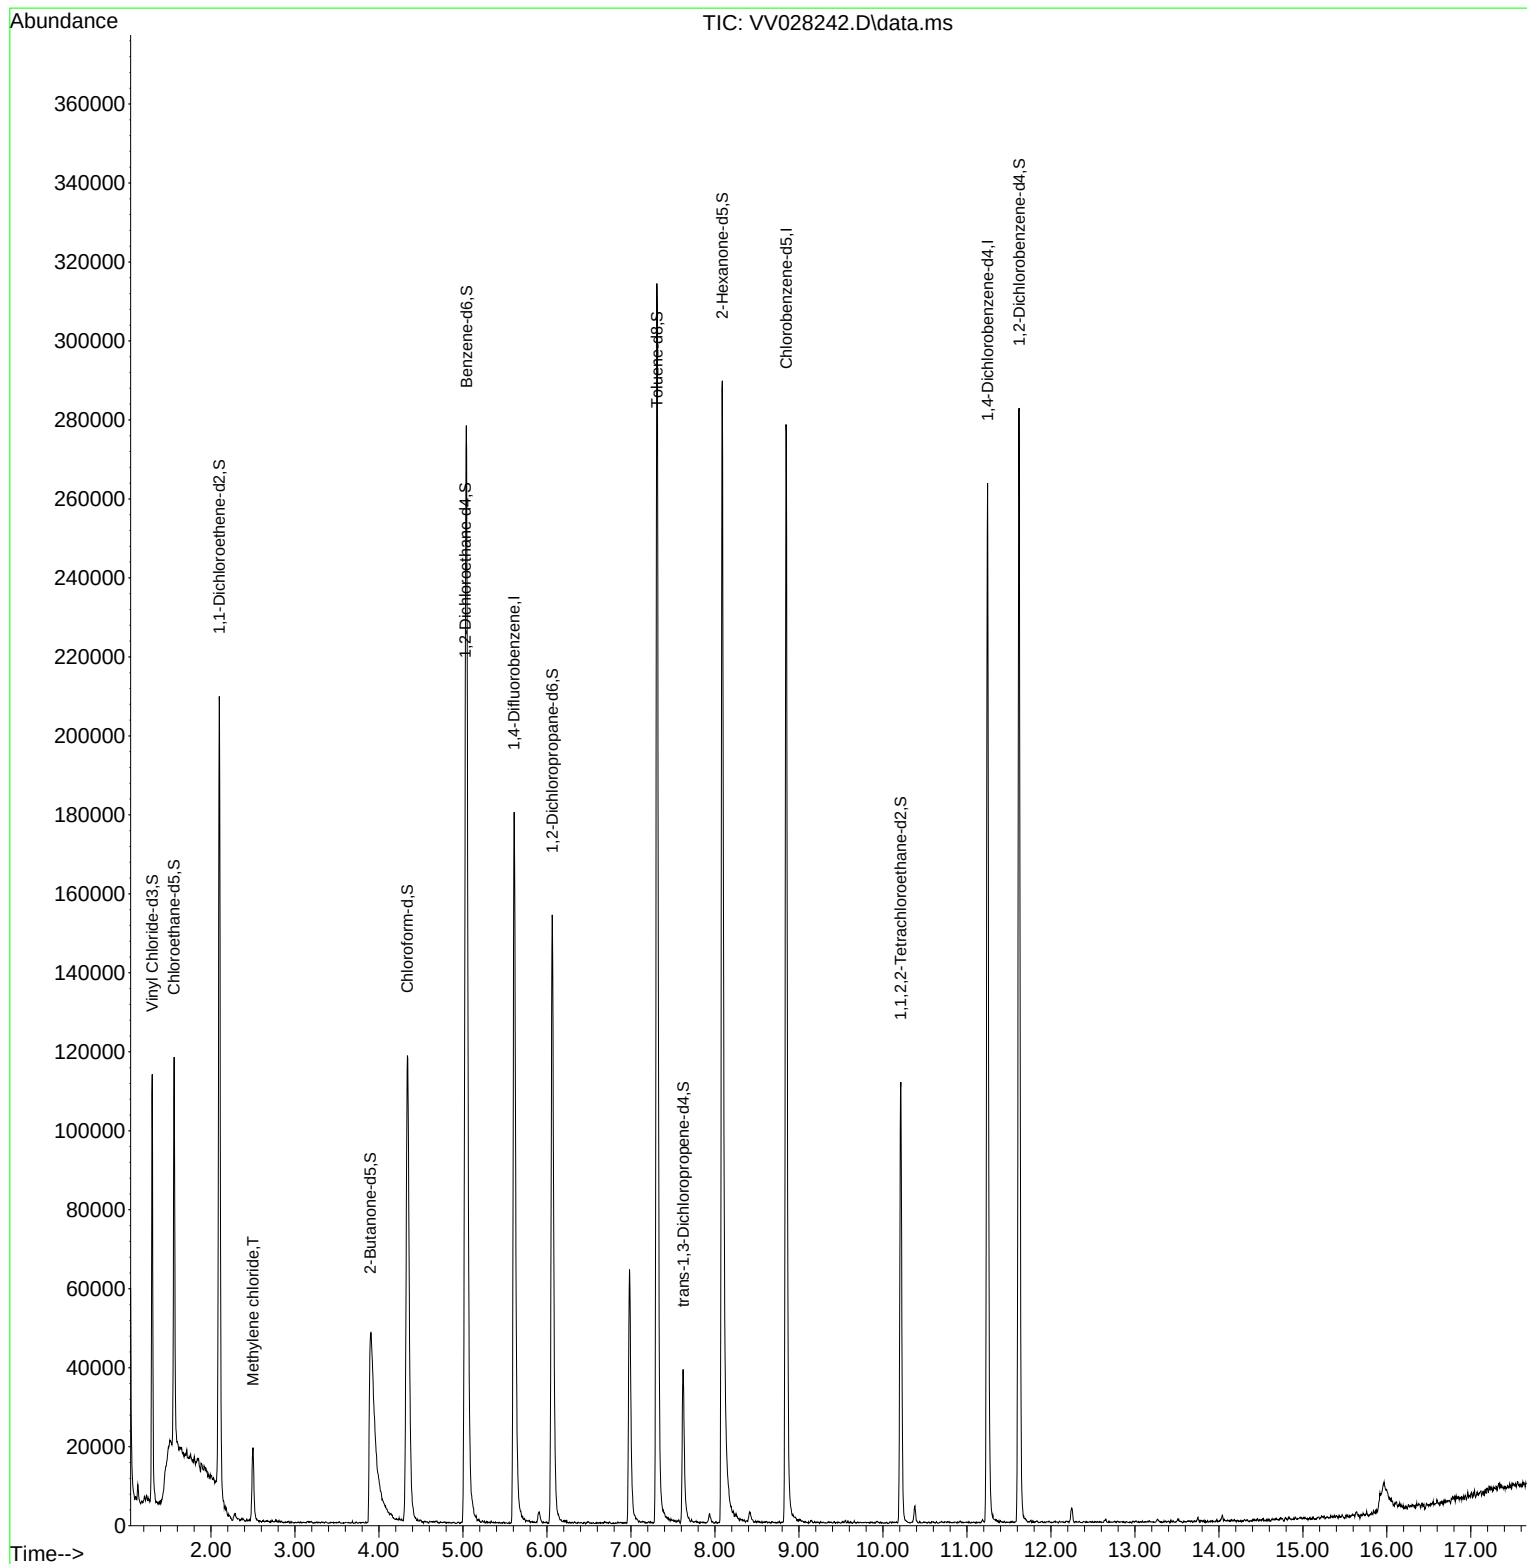

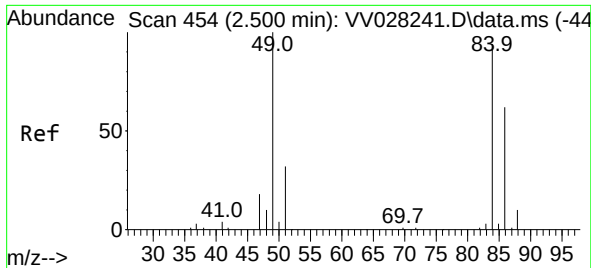

#16
Methylene chloride
Concen: 0.636 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV028242.D
Acq: 30 Sep 2022 22:06

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Tgt Ion: 84 Resp: 8122
Ion Ratio Lower Upper
84 100
86 67.9 46.8 86.8
49 103.8 87.5 162.5

