

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
 Data File : VV028254.D
 Acq On : 01 Oct 2022 03:03
 Operator : SY/MD
 Sample : N4871-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 01 04:28:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	172311	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	173177	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	84579	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	72445	4.055	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.200%
7) Chloroethane-d5	1.561	69	64875	4.568	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.400%
11) 1,1-Dichloroethene-d2	2.098	63	106702	3.444	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.800%
20) 2-Butanone-d5	3.902	46	144420	47.886	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.780%
24) Chloroform-d	4.339	84	141346	4.958	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
26) 1,2-Dichloroethane-d4	5.027	65	65295	4.814	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%
32) Benzene-d6	5.040	84	282443	4.974	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
36) 1,2-Dichloropropane-d6	6.063	67	85624	4.837	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.800%
41) Toluene-d8	7.310	98	231478	4.504	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%
43) trans-1,3-Dichloroprop...	7.622	79	24381	3.813	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.200%
46) 2-Hexanone-d5	8.088	63	120833	45.276	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.560%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	65888	5.445	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	90622	5.463	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.200%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	4973	0.374	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028254.D
Acq On : 01 Oct 2022 03:03
Operator : SY/MD
Sample : N4871-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Oct 01 04:28:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

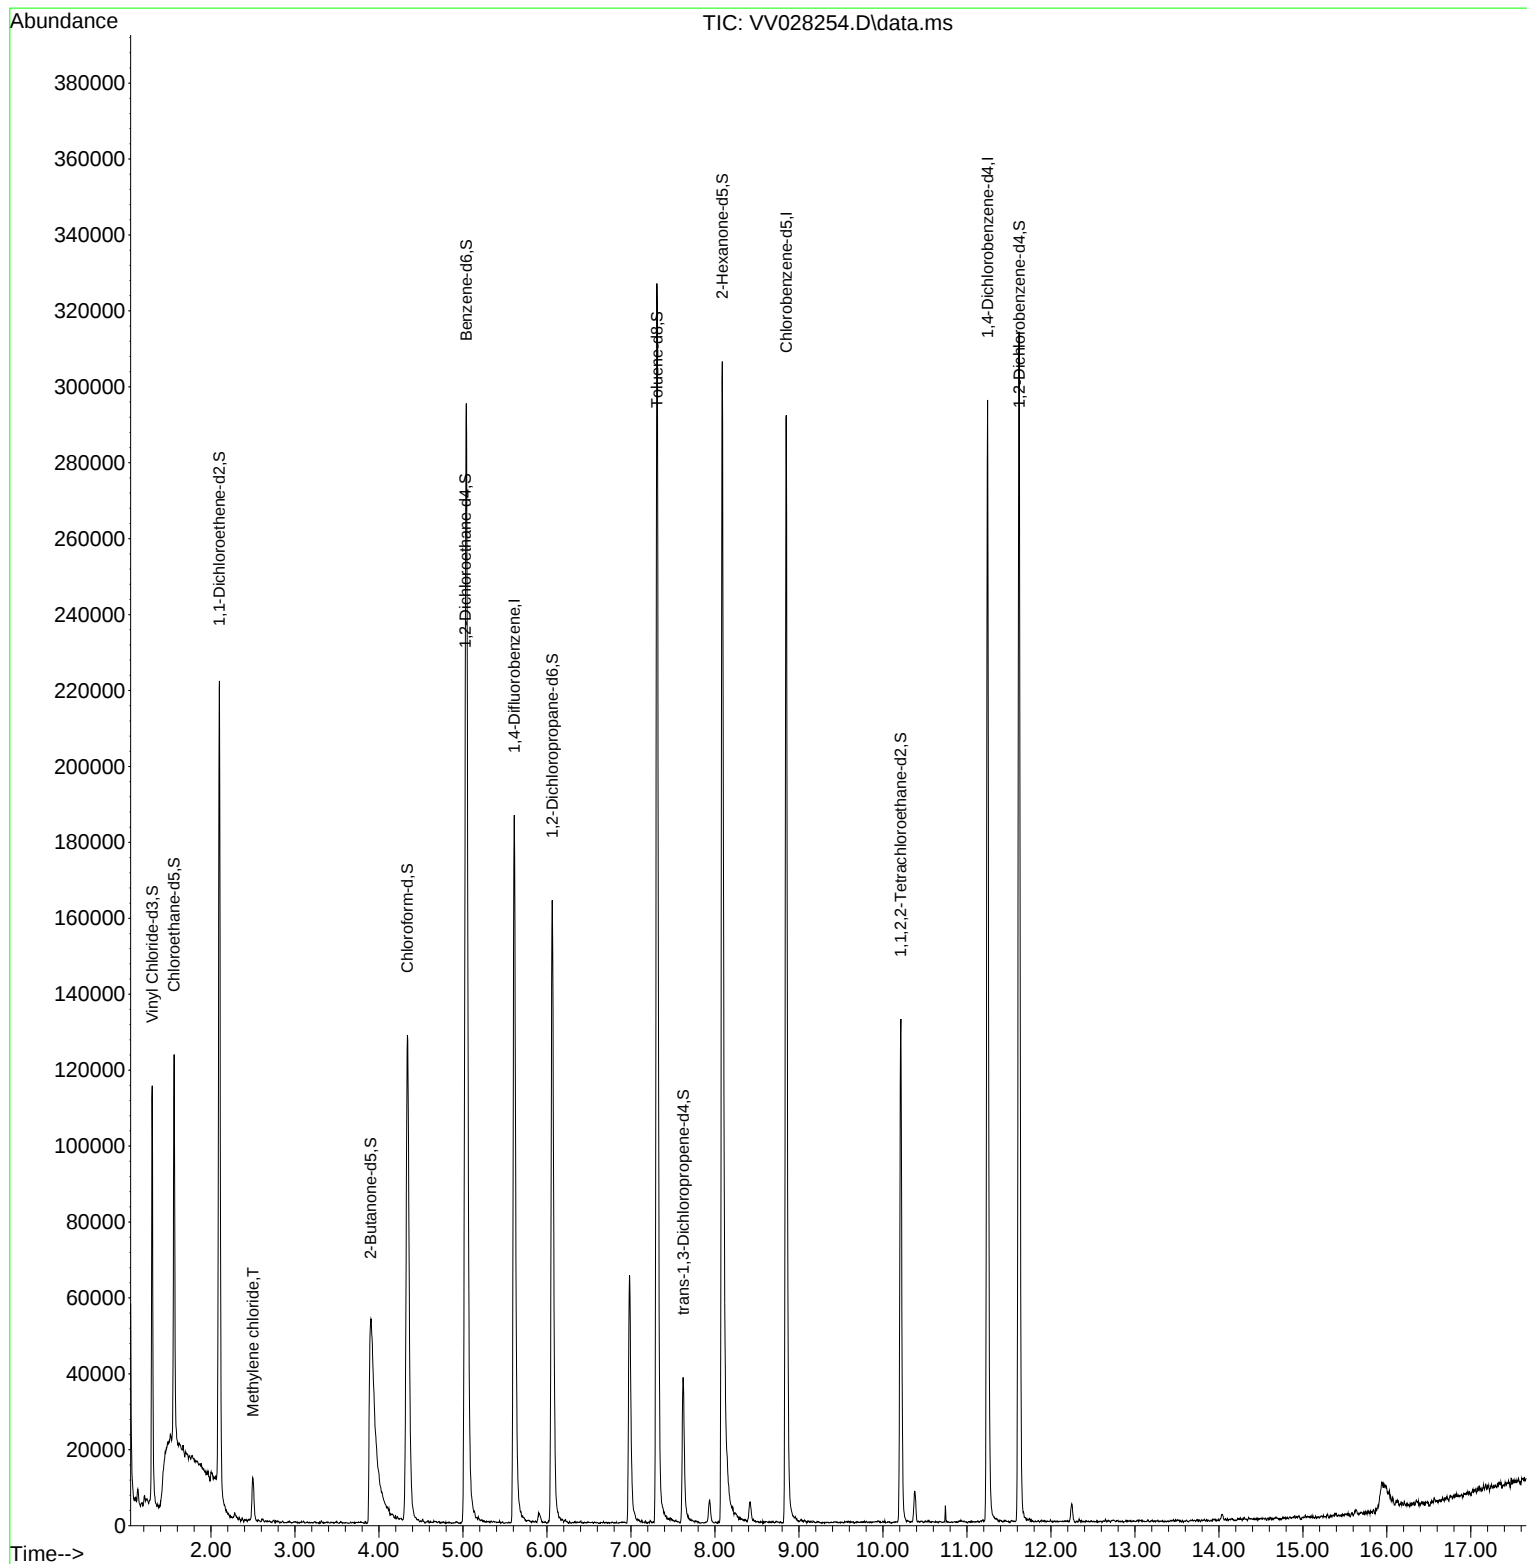

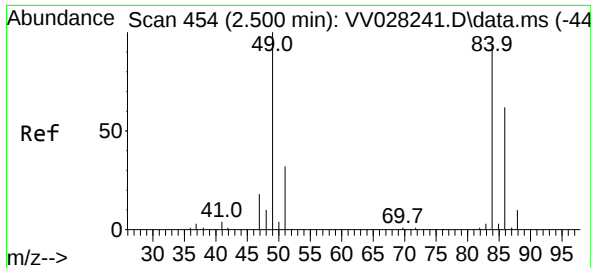

#16
Methylene chloride
Concen: 0.374 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV028254.D
Acq: 01 Oct 2022 03:03

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 4973
Ion Ratio Lower Upper
84 100
86 56.9 46.8 86.8
49 113.4 87.5 162.5

