

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
 Data File : VV028247.D
 Acq On : 01 Oct 2022 00:08
 Operator : SY/MD
 Sample : N4866-03DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXFP9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	97	rBV2	219084	241856	33.40%	4.081%
2	1.410	109	115	122	rBV	20491	26597	3.67%	0.449%
3	1.561	155	162	179	rVB	88989	108224	14.95%	1.826%
4	2.098	320	329	344	rVB	189436	276282	38.16%	4.662%
5	2.500	444	454	471	rVB2	9718	17061	2.36%	0.288%
6	2.754	525	533	545	rVB5	4469	8335	1.15%	0.141%
7	3.905	873	891	927	rBV4	89375	374174	51.68%	6.314%
8	4.339	1010	1026	1056	rBV	127849	322668	44.56%	5.445%
9	5.040	1228	1244	1272	rBV2	289624	724067	100.00%	12.219%
10	5.609	1408	1421	1446	rBV	196134	409198	56.51%	6.905%
11	6.063	1550	1562	1588	rBV	165915	346497	47.85%	5.847%
12	6.982	1838	1848	1875	rBV	69019	135645	18.73%	2.289%
13	7.310	1939	1950	1983	rBV	317705	571583	78.94%	9.645%
14	7.622	2037	2047	2078	rBV	39262	76786	10.60%	1.296%
15	7.937	2133	2145	2157	rBV3	7652	14569	2.01%	0.246%
16	8.088	2180	2192	2225	rBV	302008	618811	85.46%	10.442%
17	8.847	2416	2428	2458	rBV	302865	516648	71.35%	8.718%
18	10.214	2839	2853	2871	rBV	124633	198338	27.39%	3.347%
19	10.378	2896	2904	2917	rVB2	12052	19900	2.75%	0.336%
20	11.246	3163	3174	3196	rBV	284103	448317	61.92%	7.565%
21	11.622	3279	3291	3313	rBV	287087	462077	63.82%	7.797%
22	15.927	4620	4630	4633	rBV10	4945	8344	1.15%	0.141%




Sum of corrected areas: 5925977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028247.D
Acq On : 01 Oct 2022 00:08
Operator : SY/MD
Sample : N4866-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFP9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

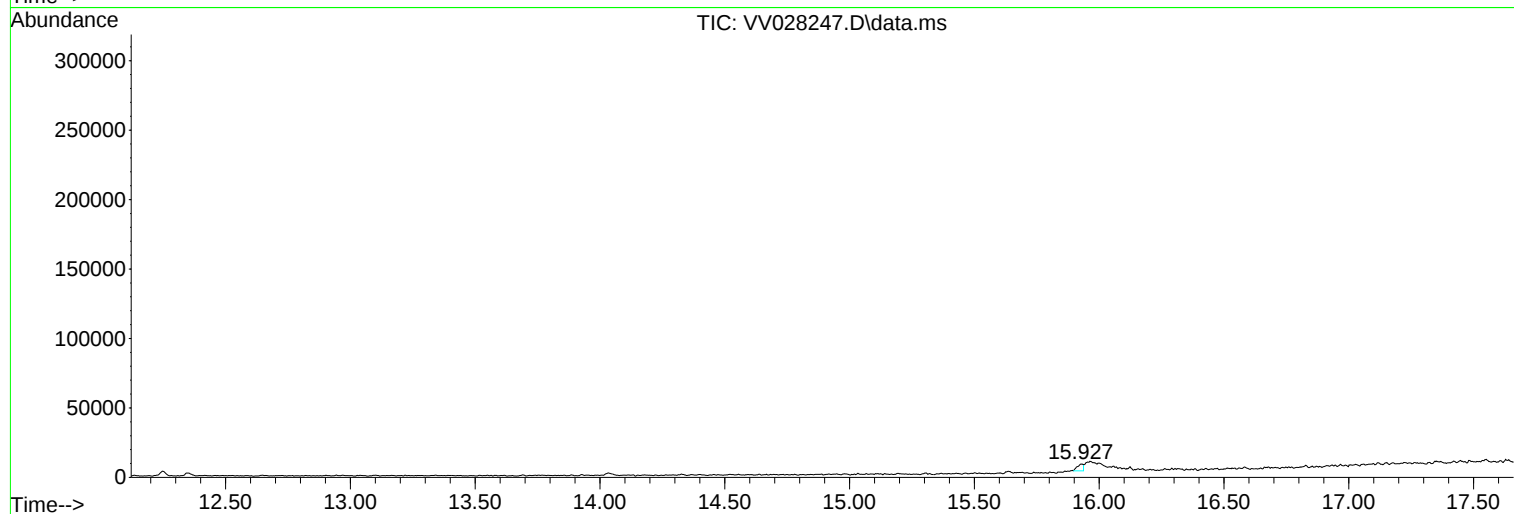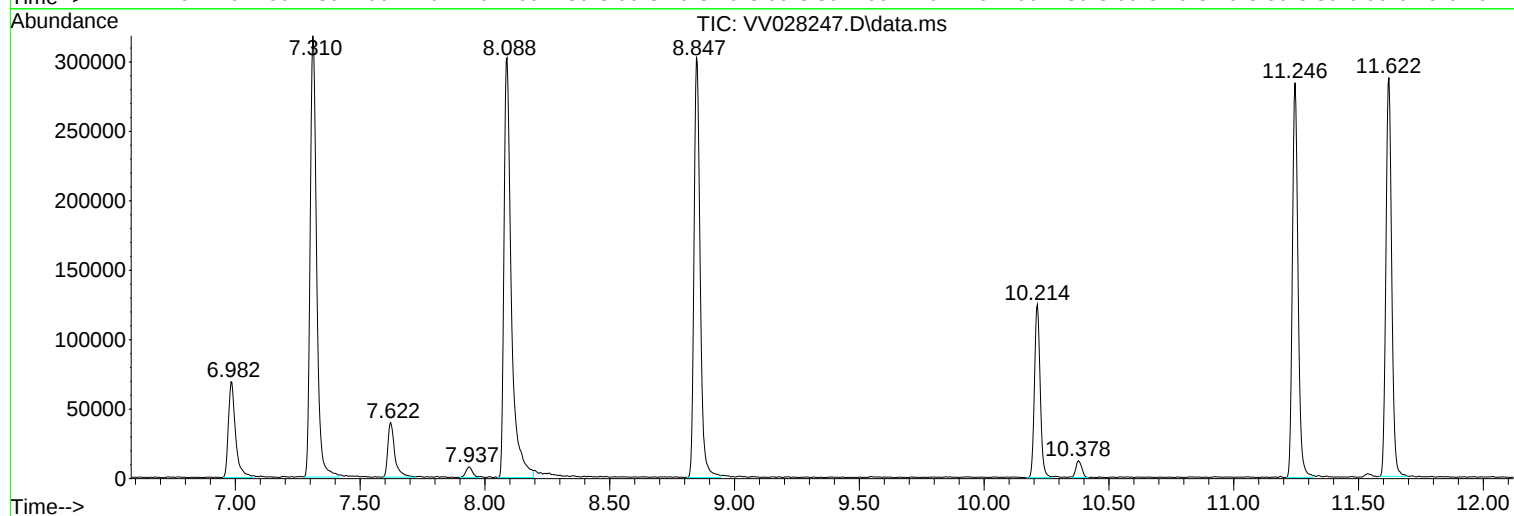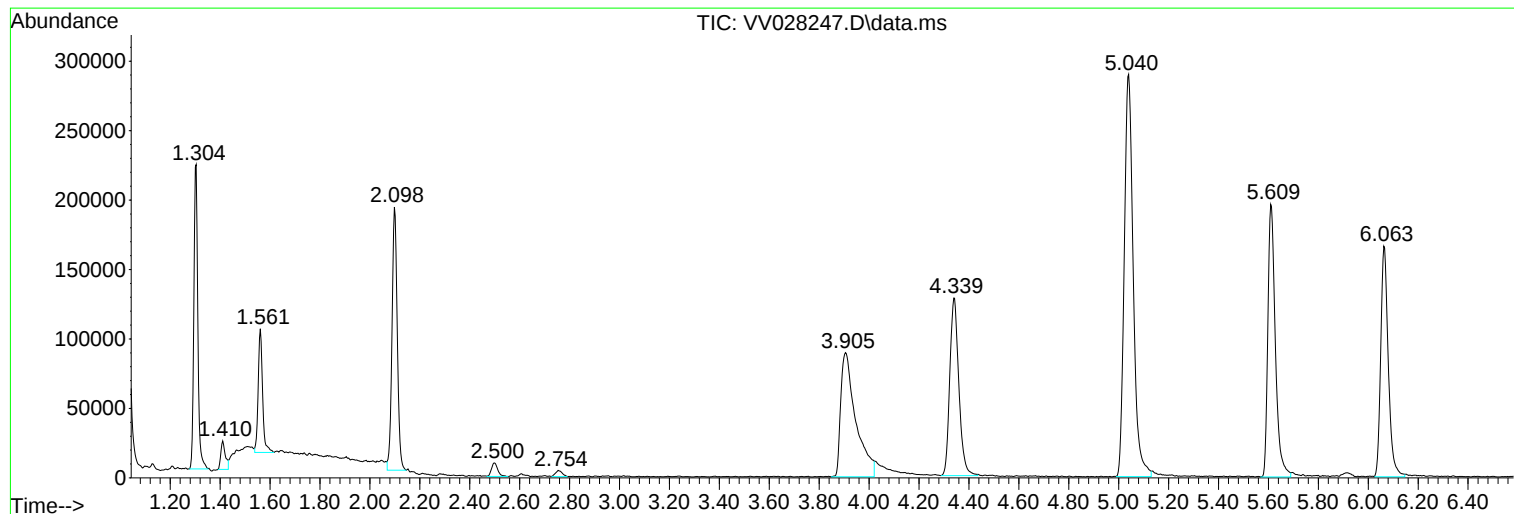

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028247.D
Acq On : 01 Oct 2022 00:08
Operator : SY/MD
Sample : N4866-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFP9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028247.D
Acq On : 01 Oct 2022 00:08
Operator : SY/MD
Sample : N4866-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFP9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc