

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
 Data File : VV028249.D
 Acq On : 01 Oct 2022 00:58
 Operator : SY/MD
 Sample : N4866-06DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXFQ2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	96	rBV2	388482	416044	41.52%	6.709%
2	1.561	155	162	173	rVB	85532	95287	9.51%	1.537%
3	2.098	319	329	348	rVB	186991	283130	28.26%	4.566%
4	2.500	444	454	463	rBV2	7045	11029	1.10%	0.178%
5	3.902	875	890	940	rBV2	340379	1002001	100.00%	16.159%
6	4.339	1009	1026	1058	rBV	113359	288113	28.75%	4.646%
7	5.040	1227	1244	1277	rBV2	251802	637725	63.65%	10.284%
8	5.612	1410	1422	1450	rBV	177396	372204	37.15%	6.002%
9	6.066	1545	1563	1588	rBV	145183	305191	30.46%	4.922%
10	6.982	1835	1848	1866	rBV	59363	113588	11.34%	1.832%
11	7.310	1939	1950	1973	rBV	284940	508514	50.75%	8.201%
12	7.622	2036	2047	2064	rBV2	35523	66271	6.61%	1.069%
13	8.088	2180	2192	2231	rBV	282365	562153	56.10%	9.066%
14	8.416	2284	2294	2306	rBV3	15326	28512	2.85%	0.460%
15	8.850	2417	2429	2457	rBV	277813	467979	46.70%	7.547%
16	10.213	2842	2853	2867	rBV	110178	175735	17.54%	2.834%
17	10.381	2895	2905	2917	rVB2	7004	11289	1.13%	0.182%
18	11.246	3162	3174	3194	rBV	273202	428054	42.72%	6.903%
19	11.622	3275	3291	3310	rBV	265410	428178	42.73%	6.905%




Sum of corrected areas: 6200997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028249.D
Acq On : 01 Oct 2022 00:58
Operator : SY/MD
Sample : N4866-06DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFQ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

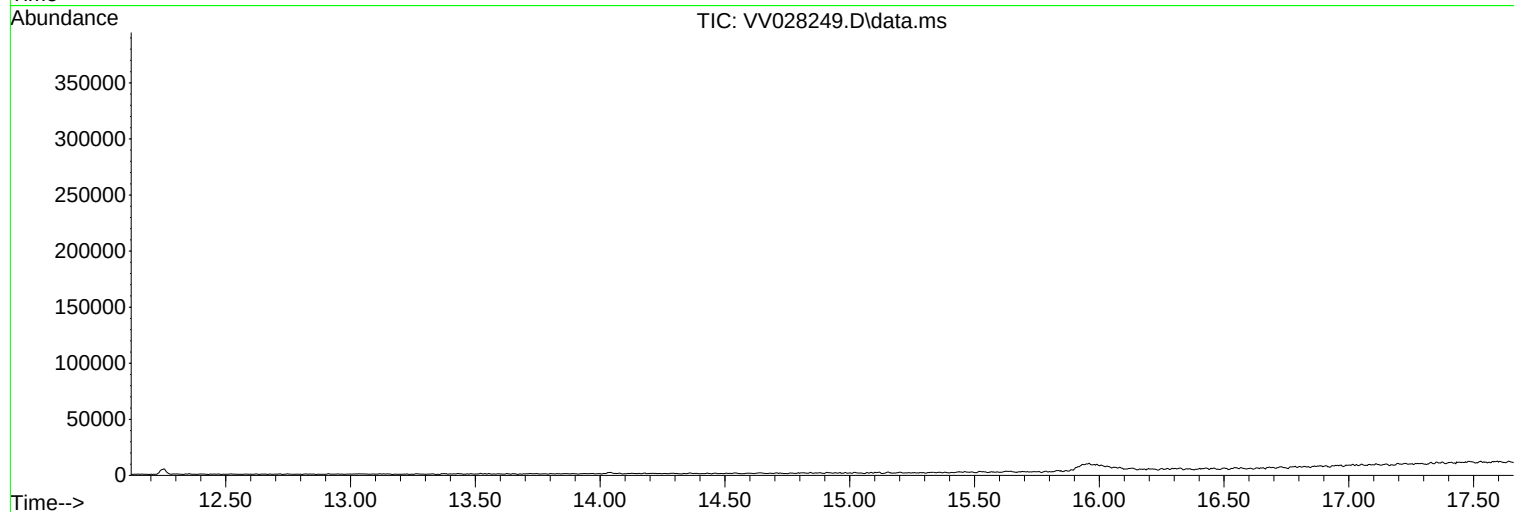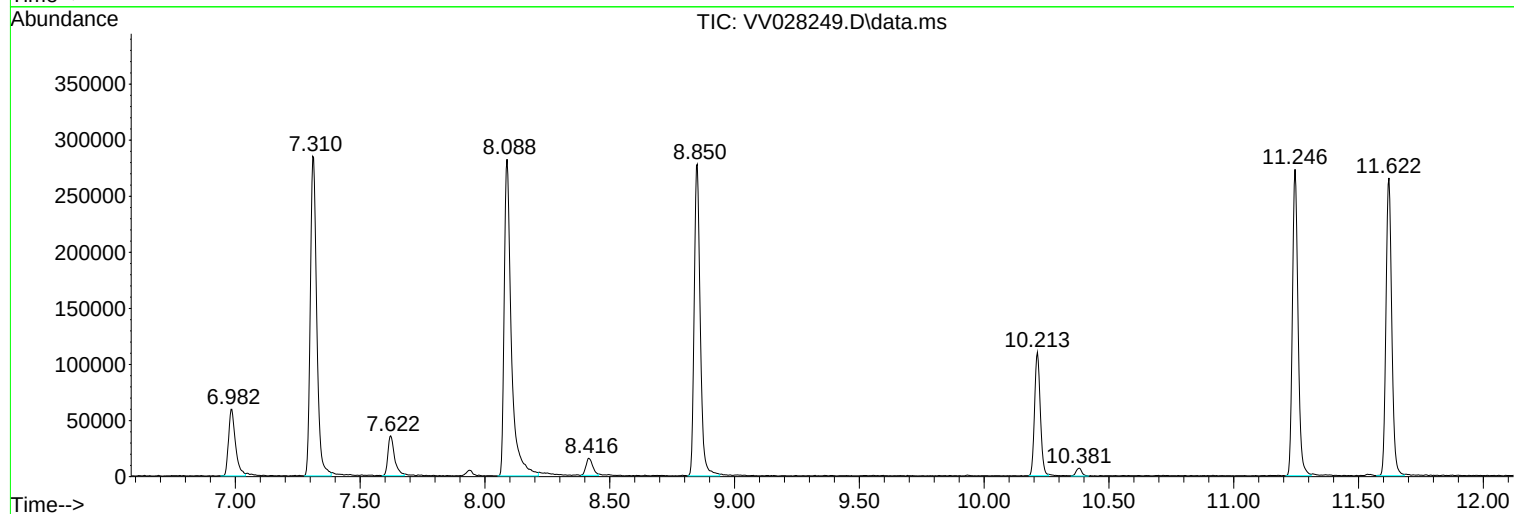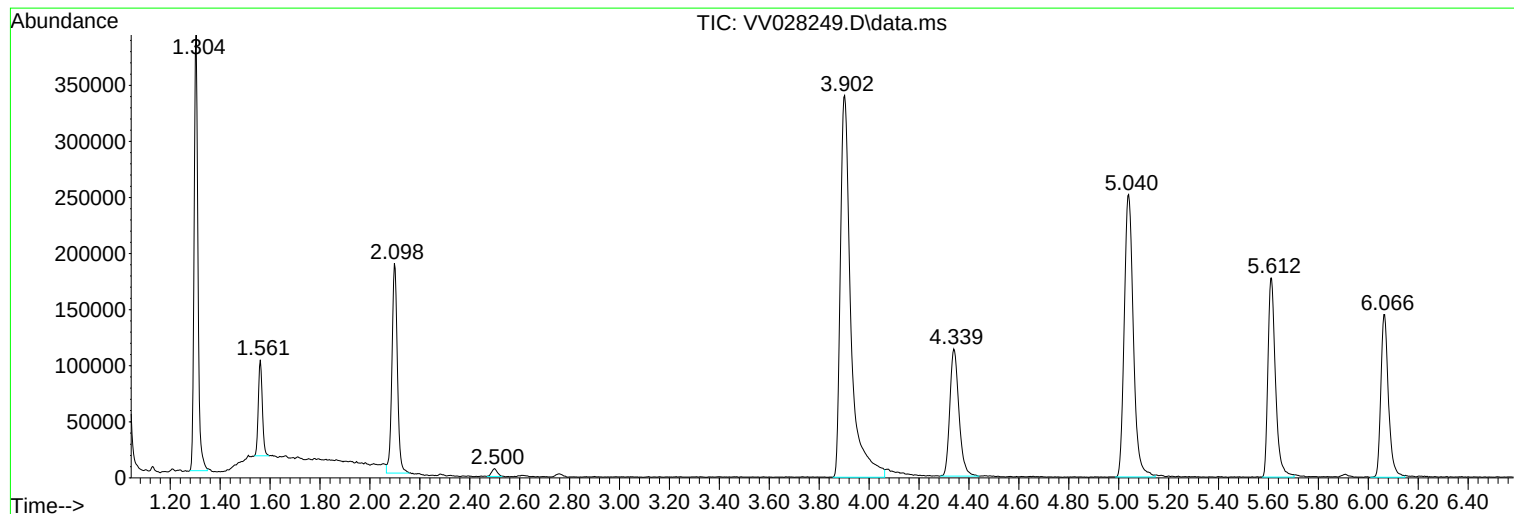

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028249.D
Acq On : 01 Oct 2022 00:58
Operator : SY/MD
Sample : N4866-06DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFQ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028249.D
Acq On : 01 Oct 2022 00:58
Operator : SY/MD
Sample : N4866-06DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFQ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc