
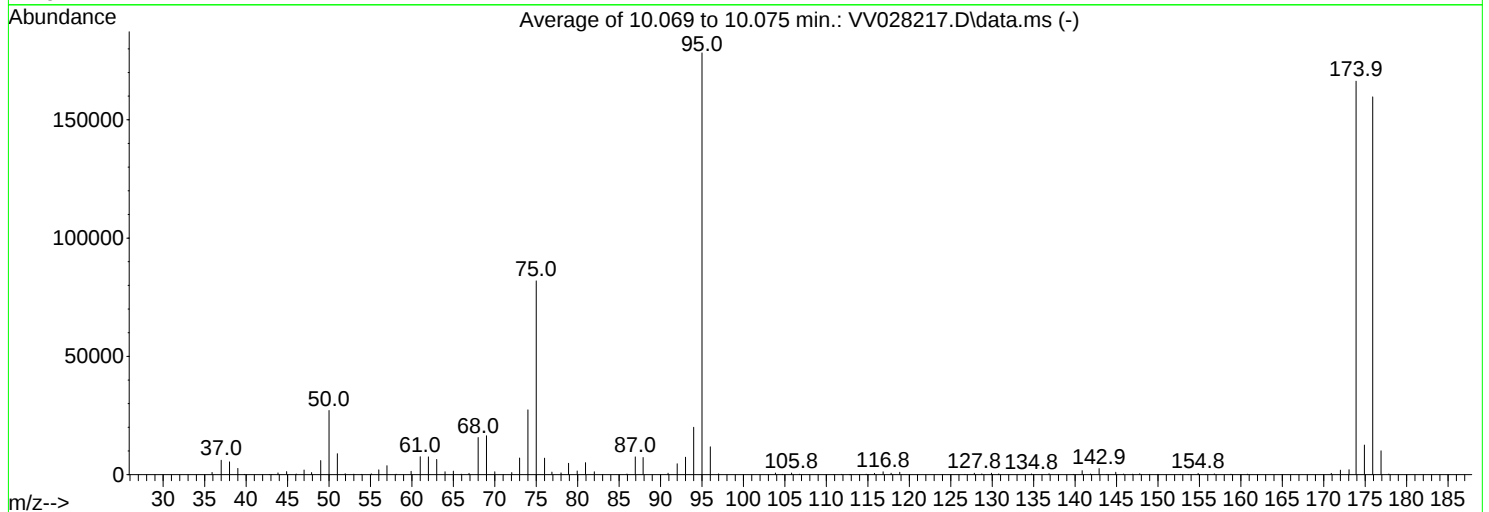


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093022\
Data File : VV028217.D
Acq On : 30 Sep 2022 09:36
Operator : SY/MD
Sample : BFB380
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB380

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 29 01:25:35 2022

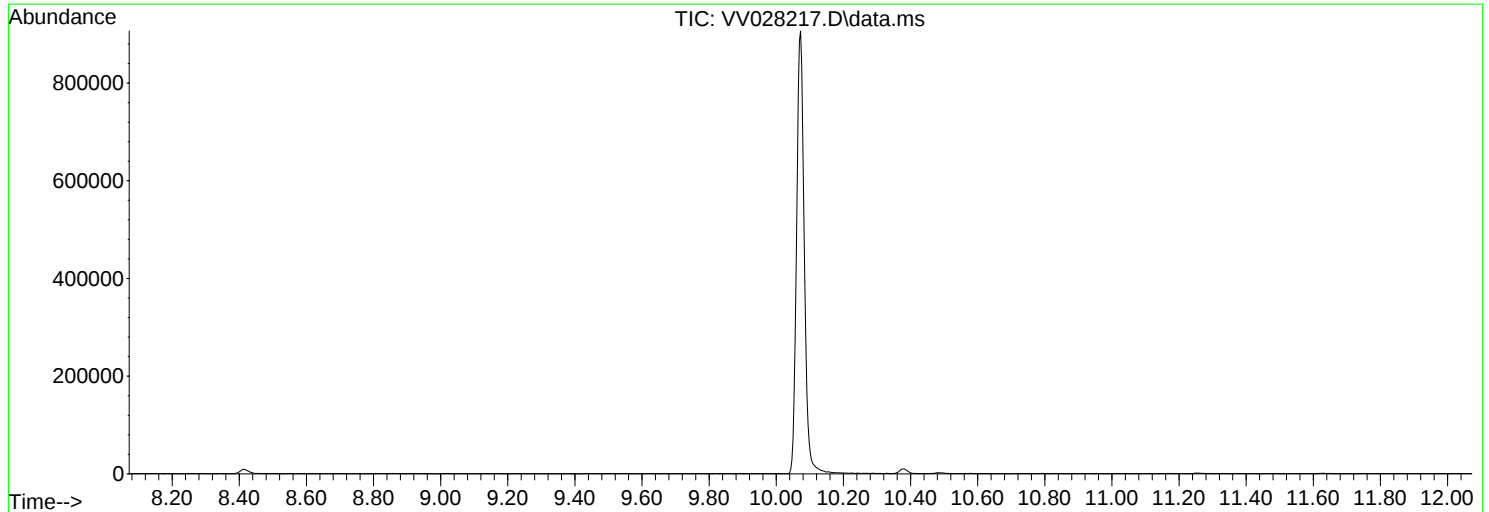

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	27096	PASS
75	95	30	80	45.9	81891	PASS
95	95	100	100	100.0	178304	PASS
96	95	5	9	6.6	11782	PASS
173	174	0.00	2	1.3	2124	PASS
174	95	50	120	93.3	166315	PASS
175	174	5	9	7.5	12494	PASS
176	174	95	105	96.0	159680	PASS
177	176	5	10	6.3	10069	PASS

m/z	Abundance
35.90	108.0
40.00	167.0
43.80	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
35.90	1136.0
37.00	6469.0
38.00	5608.0
39.00	2716.0
39.80	269.0
43.10	120.0
43.90	997.0
44.90	1341.0
46.00	295.0
47.00	2151.0
47.90	1008.0
49.00	6054.0
50.00	27696.0
51.00	8937.0
51.90	446.0
53.10	168.0
53.90	197.0
55.10	379.0
56.00	1977.0
57.00	3748.0
58.10	196.0
59.90	1486.0
61.00	7670.0
62.00	7814.0
63.00	6636.0
64.00	1368.0
65.00	1598.0
65.90	206.0
66.90	556.0
68.00	15972.0
69.00	16256.0
70.00	1246.0
72.10	832.0
73.00	7324.0
74.00	27824.0
75.00	83312.0
76.00	7048.0
76.90	1037.0
78.00	732.0
78.90	4851.0
79.90	1661.0
81.00	5351.0
82.00	1170.0
86.00	322.0
86.90	7918.0
87.90	7393.0
90.90	715.0
92.00	4718.0
93.00	7507.0
94.00	20416.0
95.00	182016.0
96.00	12327.0
97.00	380.0
103.90	602.0
105.00	230.0
105.80	729.0
106.80	211.0
110.90	170.0
111.80	103.0
114.80	163.0
115.80	498.0
116.80	1193.0
117.80	515.0
118.90	1049.0
126.70	128.0
127.90	587.0
128.80	342.0
129.90	670.0
130.80	317.0
134.70	339.0
136.90	347.0
139.80	176.0
140.90	1631.0
141.90	254.0
142.90	2803.0
143.80	188.0
144.90	1098.0
145.80	307.0
146.90	183.0
147.80	343.0
148.90	151.0
150.00	228.0
152.70	203.0
153.70	132.0
154.90	535.0
155.80	111.0
156.70	372.0
158.80	182.0
160.80	203.0
170.90	454.0
172.00	1832.0
173.00	2084.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

173.90	165952.0
174.90	12425.0
175.90	158464.0
176.90	10185.0
177.80	289.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
35.90	1073.0
37.00	6328.0
38.00	5565.0
39.00	2755.0
39.80	227.0
42.80	117.0
43.90	1025.0
44.90	1330.0
46.00	333.0
47.00	2030.0
47.90	918.0
49.00	6170.0
50.00	28104.0
51.00	9195.0
52.00	440.0
53.00	179.0
53.90	170.0
55.10	357.0
56.00	2115.0
57.00	3950.0
58.10	178.0
59.90	1482.0
61.00	7815.0
62.00	7799.0
63.00	6685.0
64.00	1217.0
65.00	1528.0
66.00	232.0
66.90	610.0
68.00	16274.0
69.00	17080.0
70.00	1201.0
71.10	101.0
72.10	876.0
73.00	7176.0
74.00	28416.0
75.00	84720.0
76.00	7223.0
76.90	1119.0
78.00	810.0
78.90	4970.0
80.00	1615.0
81.00	5264.0
82.00	1259.0
85.90	299.0
86.90	7744.0
87.90	7484.0
90.90	666.0
92.00	4754.0
93.00	7591.0
94.00	20832.0
95.00	184064.0
96.00	12215.0
97.00	409.0
103.90	698.0
104.70	179.0
105.80	715.0
106.80	187.0
110.90	127.0
111.90	110.0
112.80	107.0
114.80	187.0
115.80	560.0
116.90	1273.0
117.80	639.0
118.90	1049.0
126.70	126.0
127.80	590.0
128.70	322.0
129.90	605.0
130.80	338.0
134.70	345.0
136.90	403.0
139.80	176.0
140.90	1739.0
141.80	275.0
142.90	2639.0
143.80	179.0
144.90	1025.0
145.80	333.0
147.00	209.0
147.80	407.0
148.90	145.0
150.00	156.0
152.70	163.0
153.60	106.0
154.90	621.0
155.80	145.0
156.80	385.0
158.80	212.0
160.80	222.0
170.90	578.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

172.00	1976.0
173.00	2233.0
173.90	171840.0
174.90	12884.0
175.90	164416.0
176.90	10482.0
177.90	276.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
36.00	930.0
37.00	5502.0
38.00	5022.0
39.00	2513.0
40.10	217.0
42.80	115.0
43.90	980.0
44.90	1270.0
46.10	299.0
47.00	1807.0
47.90	766.0
49.00	5647.0
50.00	25488.0
51.00	8545.0
52.00	398.0
52.90	233.0
53.90	117.0
55.10	344.0
56.00	2056.0
57.00	3671.0
58.10	156.0
59.90	1392.0
61.00	7215.0
62.00	7002.0
63.00	6053.0
64.00	1044.0
65.00	1336.0
65.90	211.0
66.90	543.0
68.00	14789.0
69.00	16040.0
70.00	1145.0
71.00	110.0
72.00	839.0
73.00	6600.0
74.00	25896.0
75.00	77640.0
76.00	6729.0
76.90	1016.0
78.00	768.0
78.90	4542.0
80.00	1374.0
80.90	4653.0
82.00	1151.0
83.00	138.0
85.90	227.0
87.00	6952.0
87.90	6748.0
90.90	540.0
92.00	4424.0
93.00	7004.0
94.00	18864.0
95.00	168832.0
96.00	10804.0
97.00	337.0
103.80	710.0
104.70	159.0
105.80	651.0
106.70	193.0
111.90	105.0
114.80	203.0
115.80	558.0
116.90	1203.0
117.80	648.0
118.80	1027.0
126.70	114.0
127.80	643.0
128.70	297.0
129.90	528.0
130.80	294.0
134.80	327.0
136.80	388.0
139.80	131.0
140.80	1710.0
141.80	261.0
142.90	2328.0
143.90	137.0
144.90	890.0
145.90	286.0
146.90	175.0
147.80	407.0
149.00	122.0
154.80	572.0
155.80	151.0
156.90	342.0
158.80	220.0
160.80	225.0
170.90	634.0
172.00	1884.0
173.10	2056.0
173.90	161152.0
174.90	12173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

175.90	156160.0
176.90	9539.0
177.90	278.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380