

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
 Data File : VV028339.D
 Acq On : 04 Oct 2022 20:55
 Operator : SY/MD
 Sample : N4866-10 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXFQ6

Quant Time: Oct 04 23:35:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 04 02:28:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	198390	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	204807	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	92842	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	57691	3.870	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.400%
7) Chloroethane-d5	1.561	69	53606	4.248	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.000%
11) 1,1-Dichloroethene-d2	2.098	63	85604	3.047	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.000%
20) 2-Butanone-d5	3.902	46	143171	56.765	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.540%
24) Chloroform-d	4.342	84	119605	4.429	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
26) 1,2-Dichloroethane-d4	5.027	65	59582	4.759	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%
32) Benzene-d6	5.043	84	246879	4.394	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	6.066	67	76464	4.744	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.800%
41) Toluene-d8	7.313	98	199946	3.870	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.400%
43) trans-1,3-Dichloroprop...	7.622	79	24346	3.966	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.400%
46) 2-Hexanone-d5	8.088	63	112059	44.601	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.200%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	57571	4.712	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	76812	4.807	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds						
5) Vinyl chloride	1.304	62	155993	9.160	ug/L	99
16) Methylene chloride	2.500	84	8900	0.556	ug/L	94
18) trans-1,2-Dichloroethene	2.760	96	860	0.058	ug/L	90
22) cis-1,2-Dichloroethene	3.902	96	188819	12.650	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028339.D
Acq On : 04 Oct 2022 20:55
Operator : SY/MD
Sample : N4866-10 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFQ6

Quant Time: Oct 04 23:35:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 04 02:28:45 2022
Response via : Initial Calibration




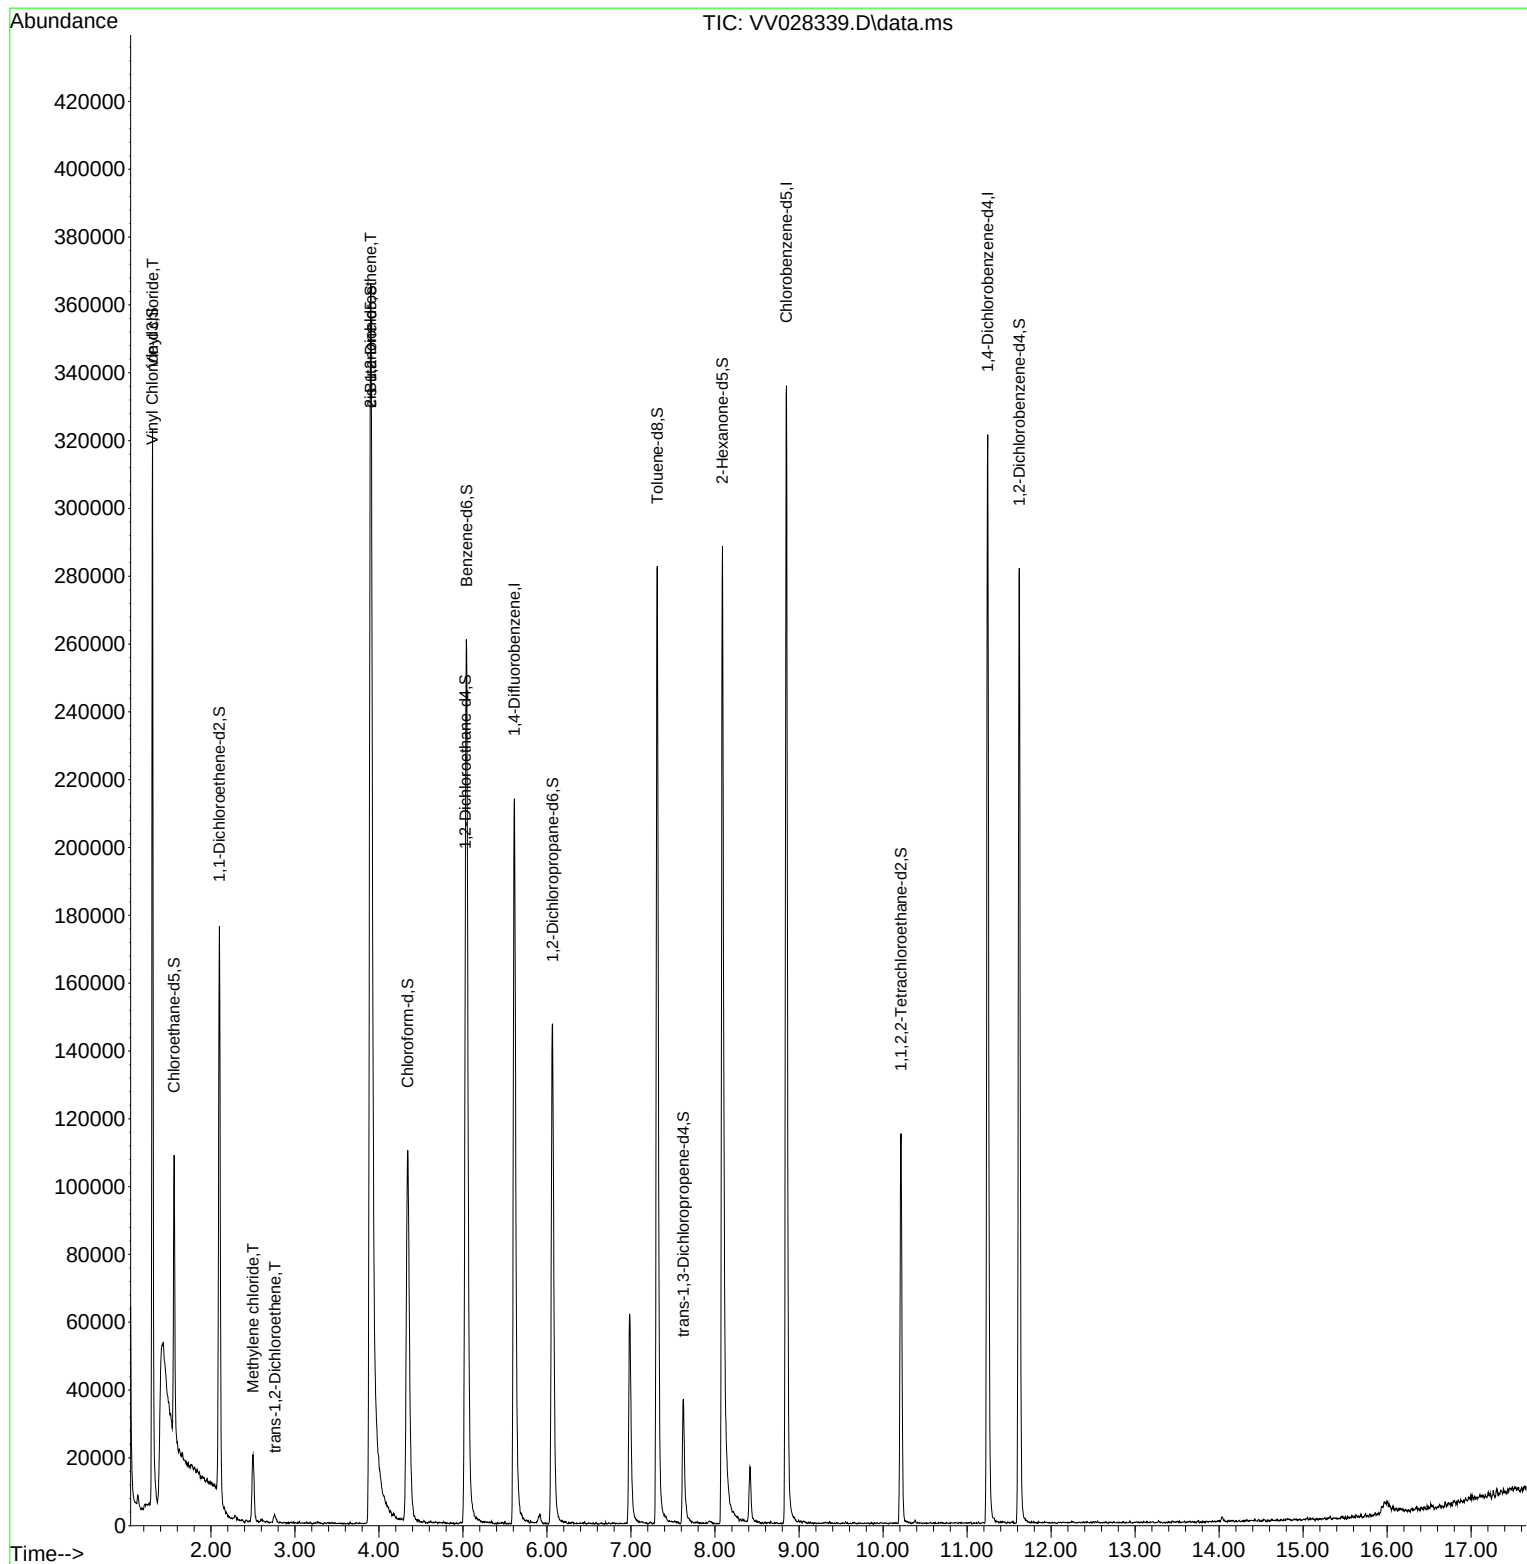


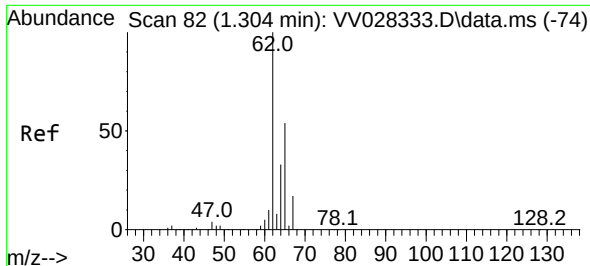

#5
 Vinyl chloride
 Concen: 9.160 ug/L
 RT: 1.304 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VV028339.D
 Acq: 04 Oct 2022 20:55




Instrument :
 MSVOA_V
 ClientSampleId :
 EXFQ6


Tgt Ion: 62 Resp: 155993
 Ion Ratio Lower Upper
 62 100
 64 33.3 23.0 42.8

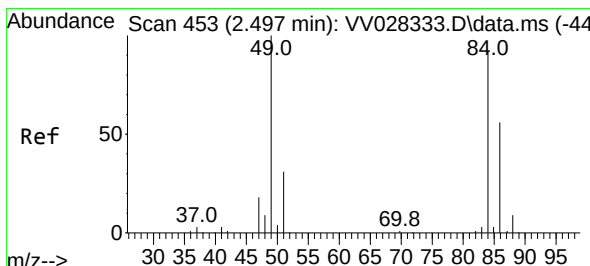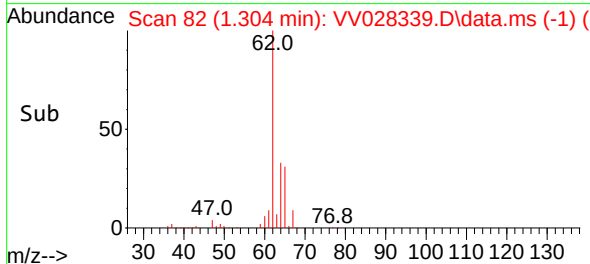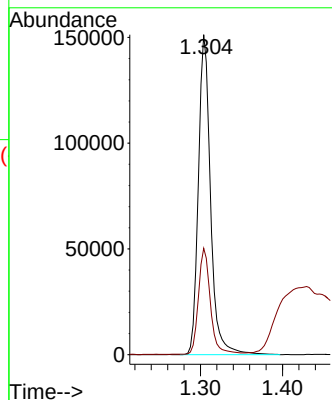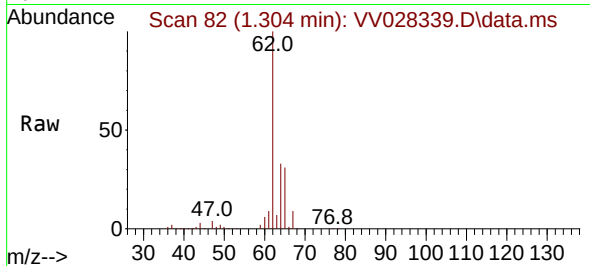

#16
 Methylene chloride
 Concen: 0.556 ug/L
 RT: 2.500 min Scan# 454
 Delta R.T. -0.000 min
 Lab File: VV028339.D
 Acq: 04 Oct 2022 20:55

Tgt Ion: 84 Resp: 8900
 Ion Ratio Lower Upper
 84 100
 86 64.4 46.8 86.8
 49 116.5 87.5 162.5


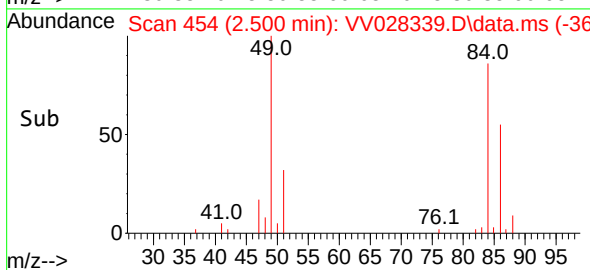
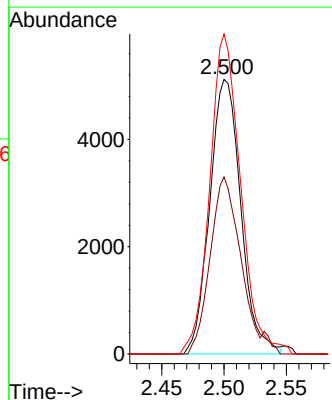
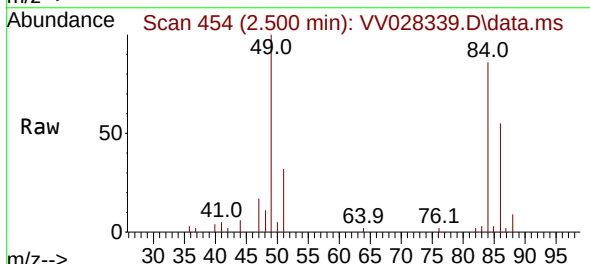


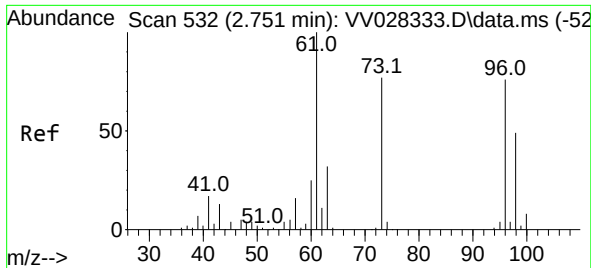

#18
trans-1,2-Dichloroethene
Concen: 0.058 ug/L
RT: 2.760 min Scan# 51
Delta R.T. 0.010 min
Lab File: VV028339.D
Acq: 04 Oct 2022 20:55

Instrument :
MSVOA_V
ClientSampleId :
EXFQ6

Tgt Ion: 96 Resp: 860
Ion Ratio Lower Upper
96 100
61 151.4 96.2 178.6
98 71.3 45.7 84.9

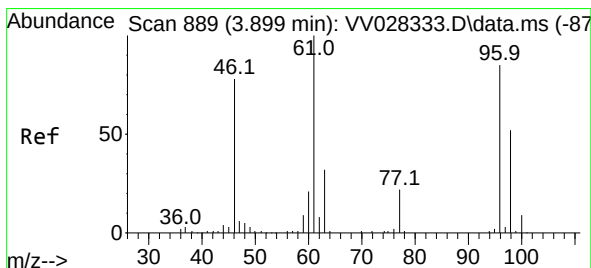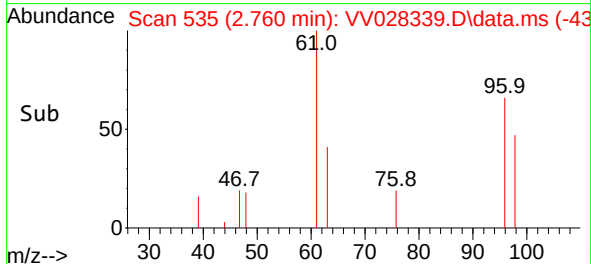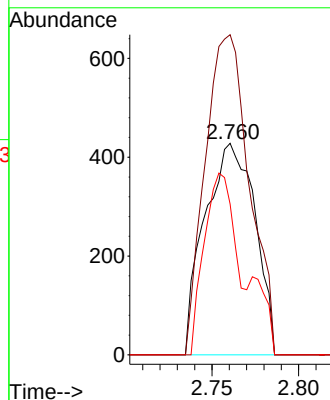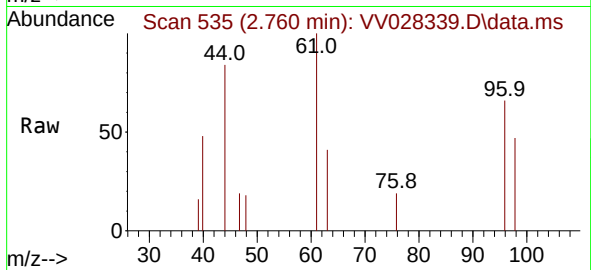

#22
cis-1,2-Dichloroethene
Concen: 12.650 ug/L
RT: 3.902 min Scan# 890
Delta R.T. -0.003 min
Lab File: VV028339.D
Acq: 04 Oct 2022 20:55

Tgt Ion: 96 Resp: 188819
Ion Ratio Lower Upper
96 100
61 121.5 87.2 161.9
68 0.0 0.0 0.0

