

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028345.D
Acq On : 04 Oct 2022 23:21
Operator : SY/MD
Sample : N4872-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX0

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Title : TRACE VOA SFAM1.0

Signal : TIC: VV028345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.876	2417	2437	2479	rBV	9690385	15884928	12.71%	5.341%
2	11.181	3137	3154	3167	rBV	25696357	40321683	32.26%	13.558%
3	11.284	3167	3186	3233	rVB3	70747895	124991967	100.00%	42.028%
4	11.654	3281	3301	3342	rBV3	64879605	116204087	92.97%	39.073%




Sum of corrected areas: 297402665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028345.D
Acq On : 04 Oct 2022 23:21
Operator : SY/MD
Sample : N4872-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

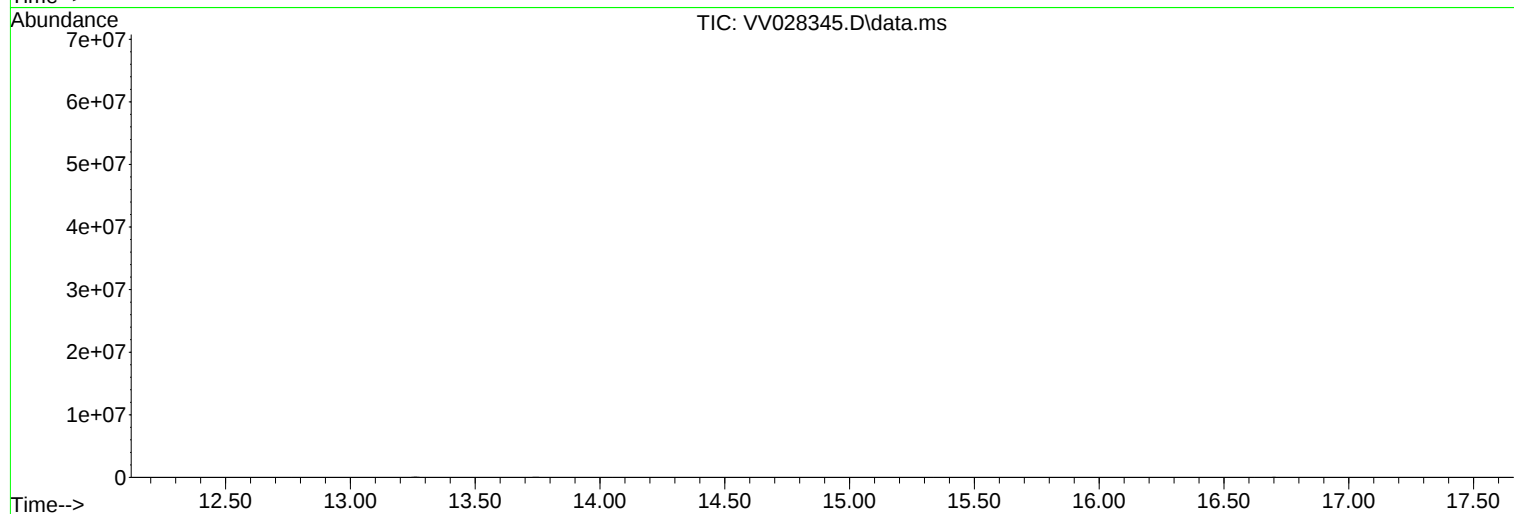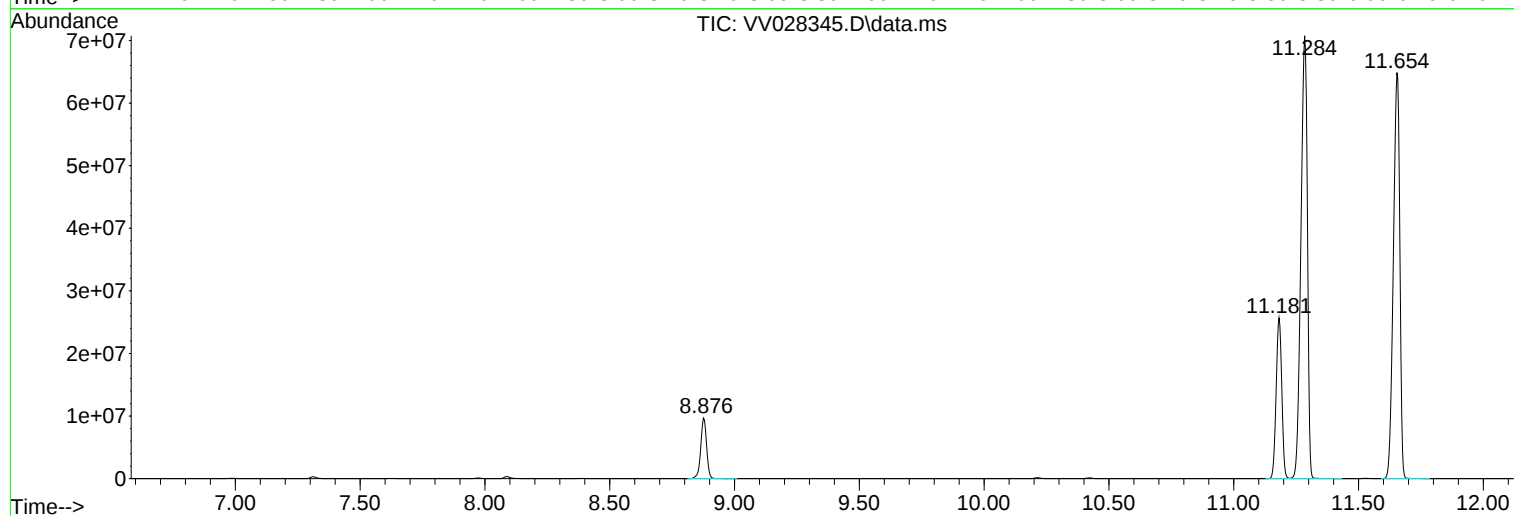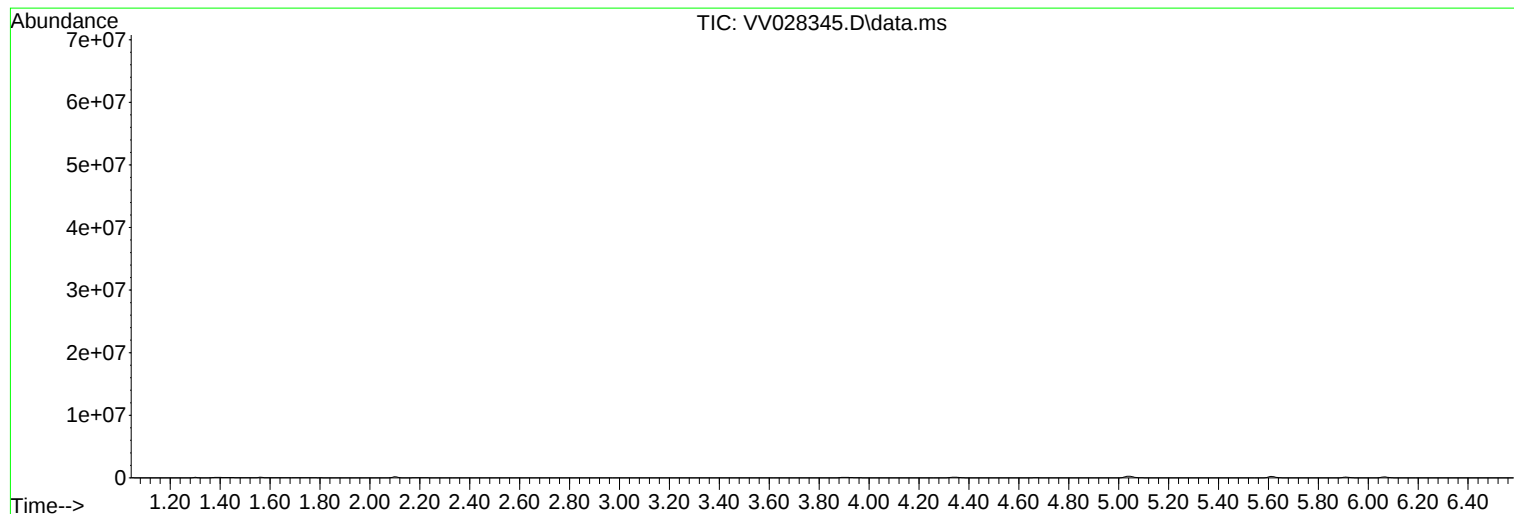

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028345.D
Acq On : 04 Oct 2022 23:21
Operator : SY/MD
Sample : N4872-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028345.D
Acq On : 04 Oct 2022 23:21
Operator : SY/MD
Sample : N4872-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc