

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028351.D
Acq On : 05 Oct 2022 01:47
Operator : SY/MD
Sample : N4872-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX6

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Title : TRACE VOA SFAM1.0

Signal : TIC: VV028351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.879	2415	2438	2476	rBV	29443781	49360869	18.23%	6.912%
2	11.194	3138	3158	3170	rBV3	69440776	131823537	48.68%	18.458%
3	11.304	3170	3192	3238	rVB5	113833679	270804540	100.00%	37.919%
4	11.673	3282	3307	3334	rBV5	109718779	262182463	96.82%	36.711%




Sum of corrected areas: 714171409

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028351.D
Acq On : 05 Oct 2022 01:47
Operator : SY/MD
Sample : N4872-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

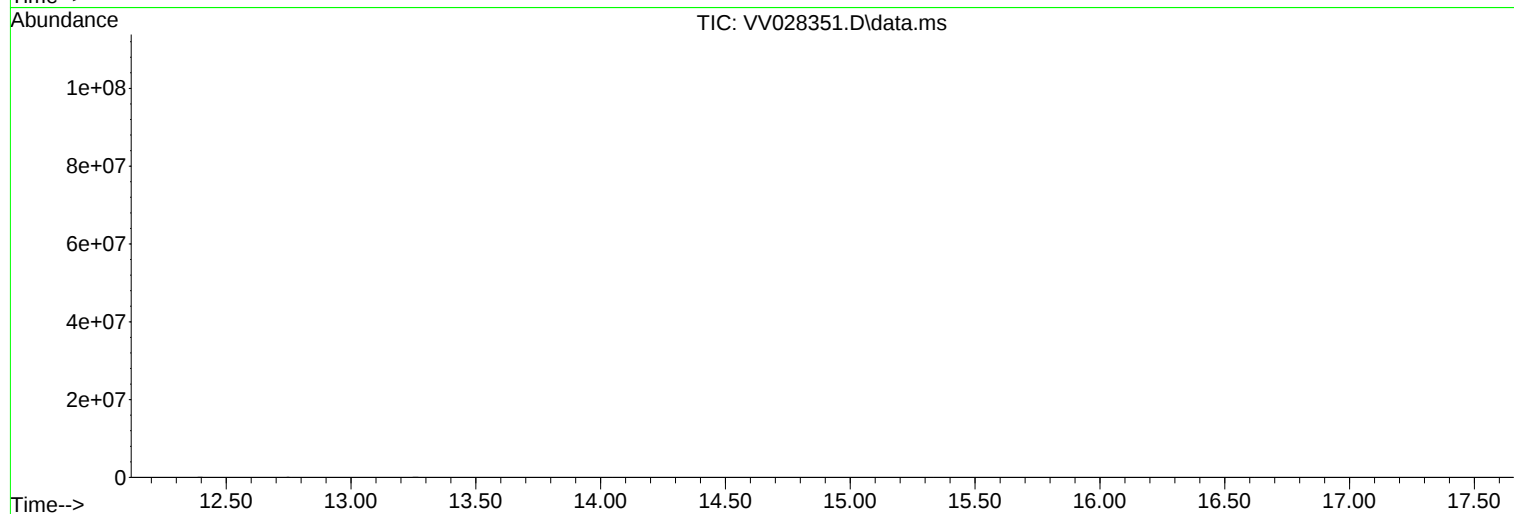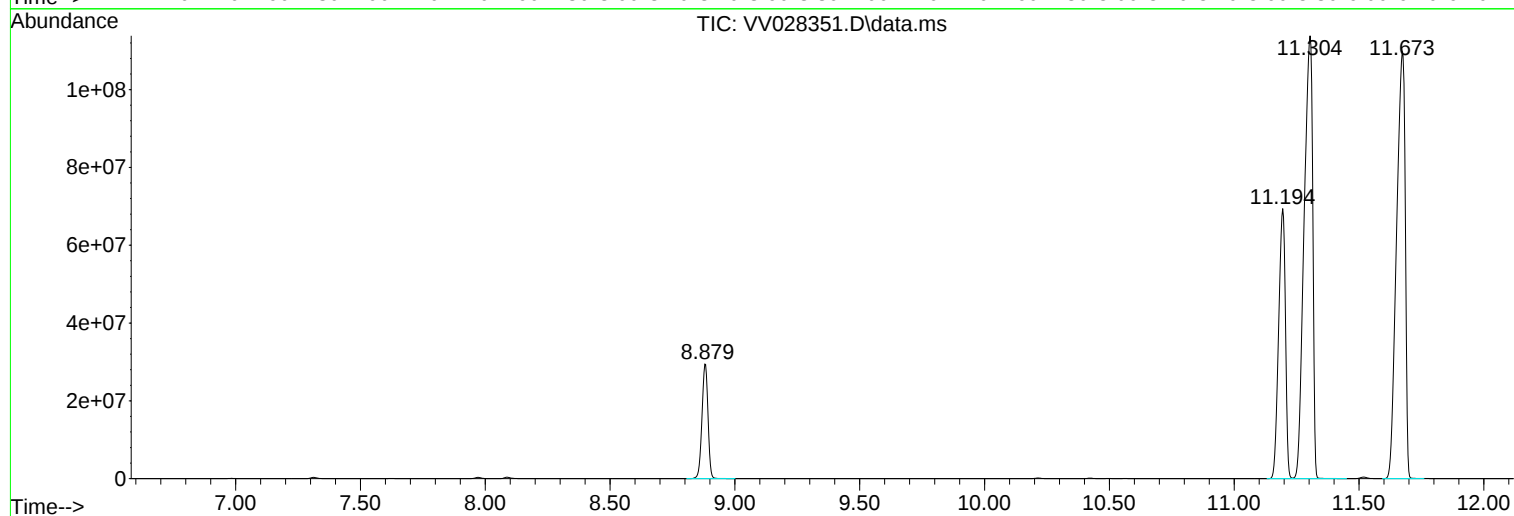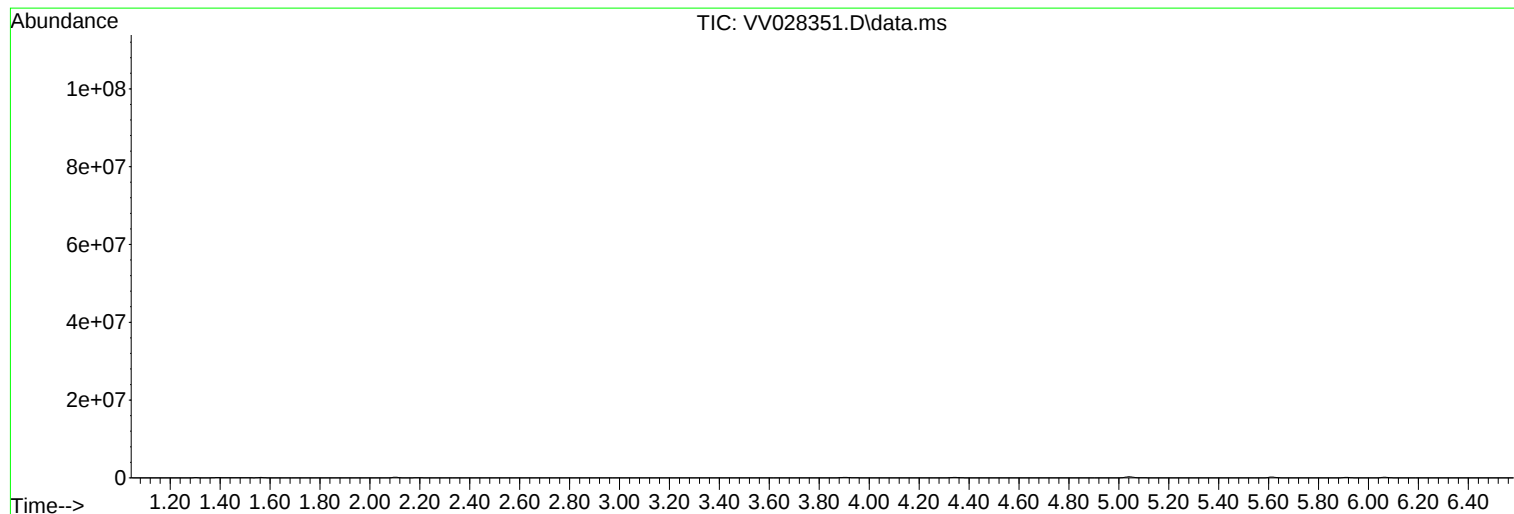

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028351.D
Acq On : 05 Oct 2022 01:47
Operator : SY/MD
Sample : N4872-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100422\
Data File : VV028351.D
Acq On : 05 Oct 2022 01:47
Operator : SY/MD
Sample : N4872-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc