
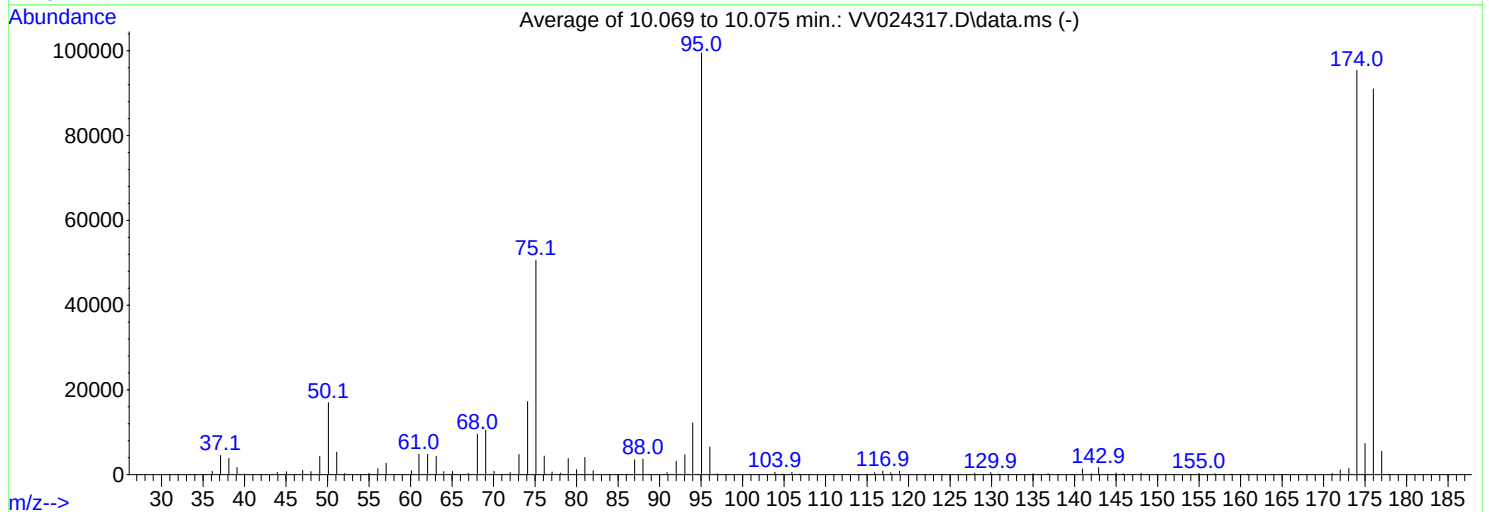


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011022\
 Data File : VV024317.D
 Acq On : 10 Jan 2022 10:21
 Operator : SY/MD
 Sample : BFB262
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB262

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Jan 11 01:51:56 2022

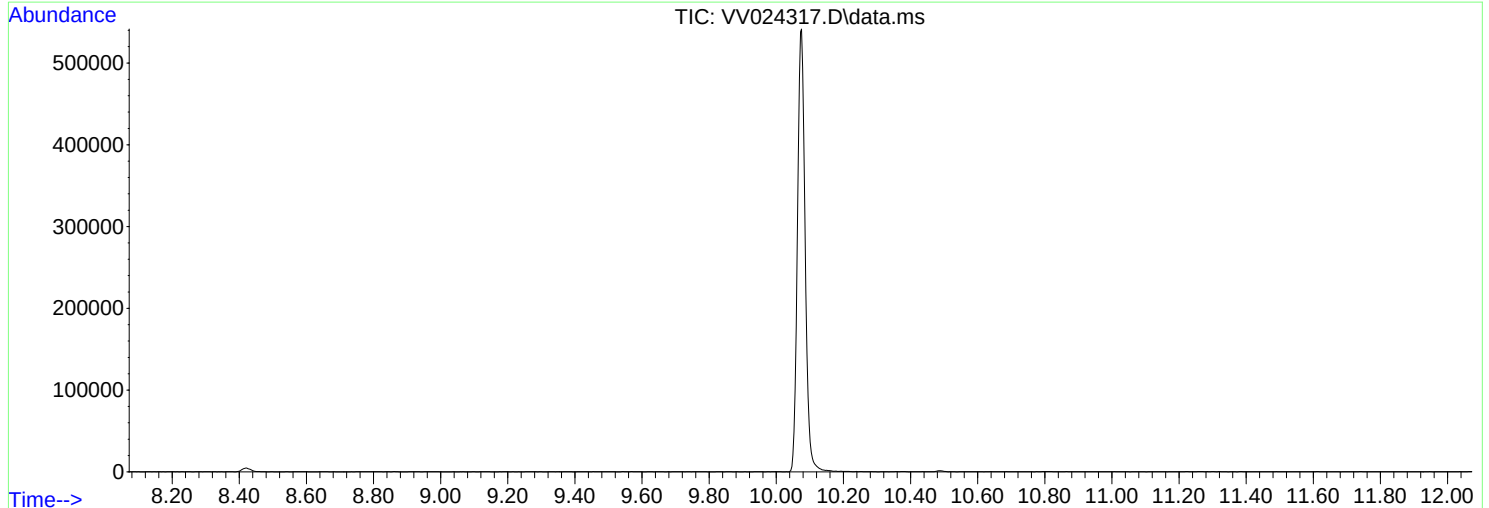

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	16977	PASS
75	95	30	80	50.8	50587	PASS
95	95	100	100	100.0	99531	PASS
96	95	5	9	6.6	6533	PASS
173	174	0.00	2	1.5	1458	PASS
174	95	50	120	95.9	95408	PASS
175	174	5	9	7.7	7353	PASS
176	174	95	105	95.4	90995	PASS
177	176	5	10	6.1	5519	PASS

m/z	Abundance
36.10	851.0
37.10	4676.0
38.10	3770.0
39.10	1744.0
40.00	164.0
44.00	756.0
45.00	655.0
46.10	140.0
47.00	1055.0
48.00	646.0
49.10	4379.0
50.10	17480.0
51.10	5464.0
52.00	296.0
55.00	330.0
56.00	1560.0
57.10	2609.0
58.20	126.0
60.10	866.0
61.00	4842.0
62.10	5066.0
63.10	4358.0
64.00	711.0
65.00	780.0
66.00	143.0
66.90	377.0
68.00	9662.0
69.10	10857.0
70.00	800.0
72.00	505.0
73.10	4847.0
74.10	17952.0
75.10	51856.0
76.10	4691.0
77.10	561.0
78.00	341.0
79.00	3985.0
80.00	1167.0
81.00	4150.0
82.00	1022.0
82.90	103.0
86.10	266.0
87.00	3743.0
88.00	3626.0
90.90	487.0
92.00	3119.0
93.00	5122.0
94.00	12938.0
95.00	102184.0
96.10	6819.0
97.00	209.0
103.90	561.0
104.80	161.0
105.90	529.0
106.90	108.0
110.00	135.0
110.90	138.0
112.10	112.0
112.80	128.0
114.90	154.0
115.90	485.0
116.90	870.0
117.80	503.0
118.90	836.0
124.00	110.0
127.90	355.0
129.00	198.0
129.90	540.0
130.80	214.0
135.00	287.0
136.80	260.0
139.60	107.0
140.90	1443.0
142.00	257.0
142.90	1738.0
143.90	138.0
145.00	407.0
145.90	228.0
146.90	131.0
148.00	349.0
149.90	124.0
151.80	118.0
154.00	116.0
155.00	344.0
156.90	274.0
158.90	167.0
160.80	120.0
171.10	247.0
172.00	1089.0
173.10	1575.0
174.00	100712.0
175.00	7697.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

176.00	96632.0
177.00	5893.0
177.90	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.10	812.0
37.10	4700.0
38.10	3972.0
39.10	1745.0
40.00	200.0
44.00	701.0
45.00	669.0
46.10	141.0
47.00	1078.0
48.00	753.0
49.10	4504.0
50.10	17584.0
51.10	5405.0
52.00	270.0
53.00	102.0
55.00	337.0
56.00	1474.0
57.00	2789.0
58.20	122.0
60.10	975.0
61.00	4995.0
62.10	4936.0
63.10	4451.0
64.00	747.0
65.00	799.0
66.00	140.0
67.00	315.0
68.10	9939.0
69.10	10853.0
70.10	805.0
72.00	487.0
73.00	4868.0
74.10	17792.0
75.10	52184.0
76.10	4531.0
77.00	678.0
78.10	387.0
79.00	3917.0
80.00	1235.0
81.00	4209.0
82.00	981.0
82.90	113.0
86.10	197.0
87.00	3642.0
88.00	3784.0
90.90	518.0
92.00	3249.0
93.10	4785.0
94.00	12558.0
95.10	103160.0
96.10	6721.0
96.90	237.0
103.90	587.0
104.80	202.0
106.00	582.0
106.80	119.0
110.20	102.0
110.90	116.0
112.10	107.0
112.90	105.0
114.90	177.0
115.90	451.0
116.90	844.0
117.80	465.0
118.90	839.0
124.10	108.0
128.00	358.0
129.00	169.0
129.90	515.0
130.90	193.0
135.00	285.0
136.80	279.0
139.70	127.0
140.90	1418.0
142.10	215.0
142.90	1745.0
143.90	172.0
145.00	443.0
145.90	230.0
146.90	121.0
148.00	370.0
149.90	115.0
151.80	112.0
154.00	124.0
155.00	310.0
156.90	305.0
159.00	161.0
160.90	123.0
171.00	285.0
172.00	1132.0
173.00	1506.0
174.00	98328.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

175.00	7628.0
176.00	94120.0
177.00	5645.0
177.90	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.10	742.0
37.10	4260.0
38.10	3760.0
39.10	1590.0
40.00	168.0
44.00	579.0
45.10	676.0
46.10	106.0
47.00	933.0
48.00	739.0
49.00	4027.0
50.10	15866.0
51.10	5057.0
52.10	264.0
55.00	313.0
56.10	1284.0
57.10	2605.0
60.10	985.0
61.00	4694.0
62.00	4421.0
63.10	4082.0
64.00	681.0
65.10	746.0
66.00	118.0
67.00	254.0
68.10	9117.0
69.00	9703.0
70.10	774.0
72.00	478.0
73.10	4505.0
74.10	16070.0
75.10	47720.0
76.10	3946.0
77.00	654.0
78.10	347.0
79.00	3495.0
80.00	1090.0
81.00	3837.0
82.00	869.0
83.00	114.0
87.00	3203.0
88.00	3589.0
90.90	460.0
92.00	3141.0
93.10	4206.0
94.00	11057.0
95.10	93248.0
96.00	6060.0
96.90	220.0
103.90	544.0
104.80	198.0
106.00	563.0
106.80	125.0
114.90	164.0
115.90	386.0
116.90	776.0
117.90	386.0
118.90	766.0
128.00	332.0
129.00	125.0
129.90	426.0
130.80	183.0
135.00	271.0
136.80	273.0
139.80	134.0
141.00	1232.0
142.10	176.0
142.90	1478.0
144.00	152.0
145.00	431.0
145.80	206.0
148.00	310.0
149.90	101.0
155.00	264.0
156.90	282.0
159.00	130.0
160.90	128.0
171.00	295.0
172.00	1019.0
173.00	1292.0
174.00	87184.0
175.00	6735.0
176.00	82232.0
177.00	5019.0
177.80	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
43.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262