




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
 Data File : VV024328.D
 Acq On : 12 Jan 2022 12:58
 Operator : SY/MD
 Sample : VV0112WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK291

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 13 03:28:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

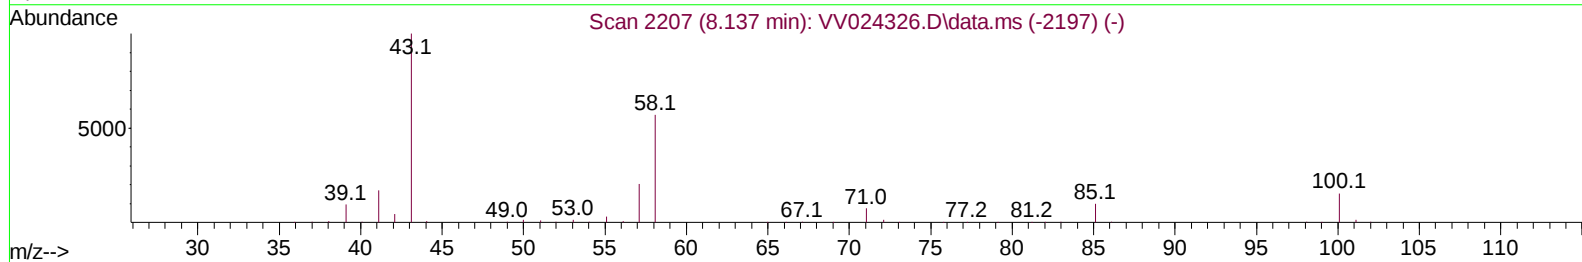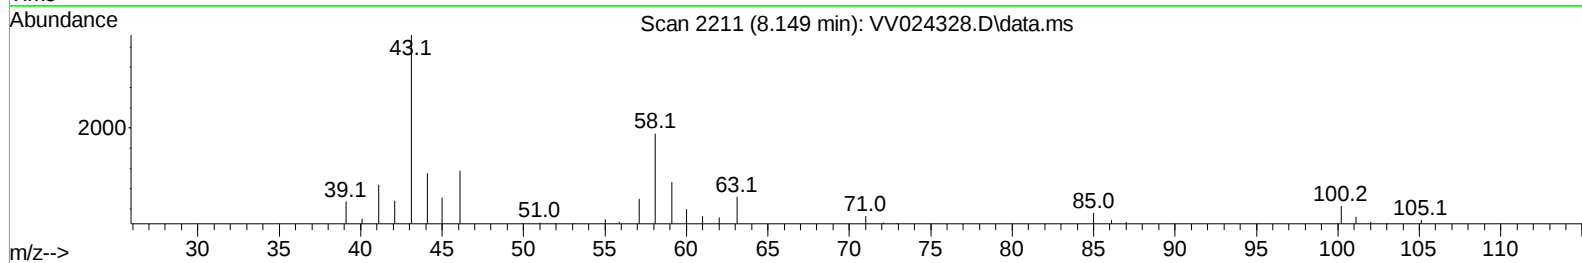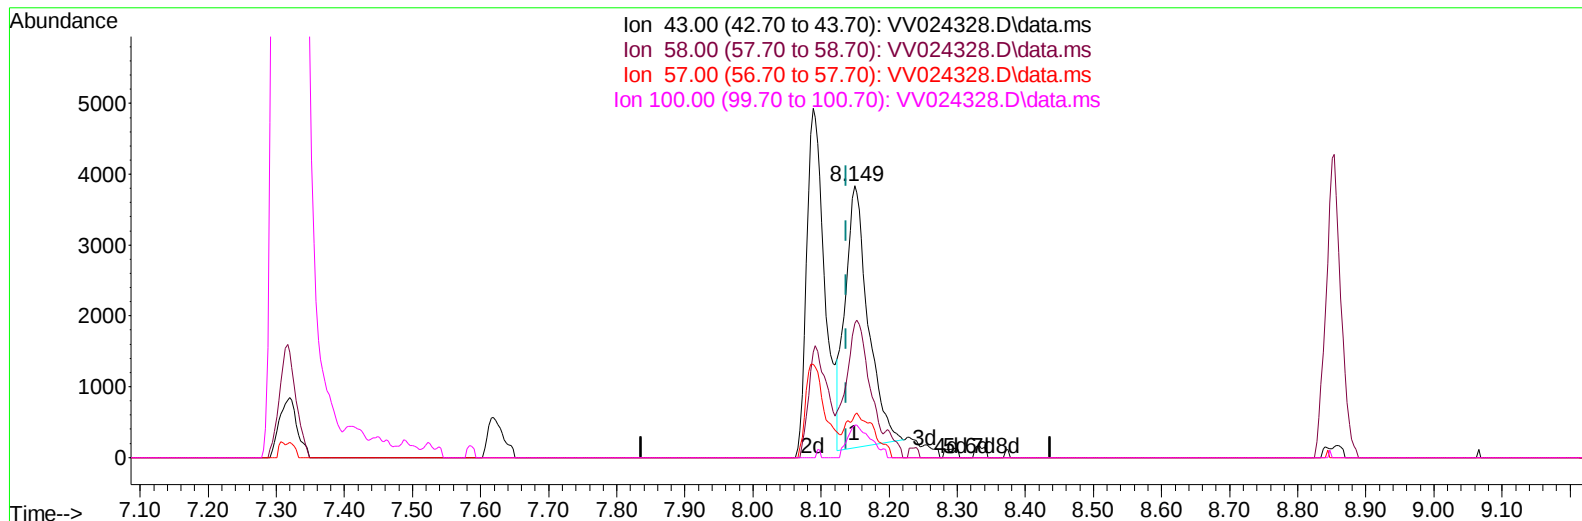

TIC: VV024328.D\data.ms

(48) 2-Hexanone (T)

8.149min (+ 0.013) 5.43 ug/L

response 8596

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	56.20	51.66
57.00	21.10	2.22#
100.00	16.20	12.15#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
 Data File : VV024328.D
 Acq On : 12 Jan 2022 12:58
 Operator : SY/MD
 Sample : VV0112WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK291

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 13 03:28:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

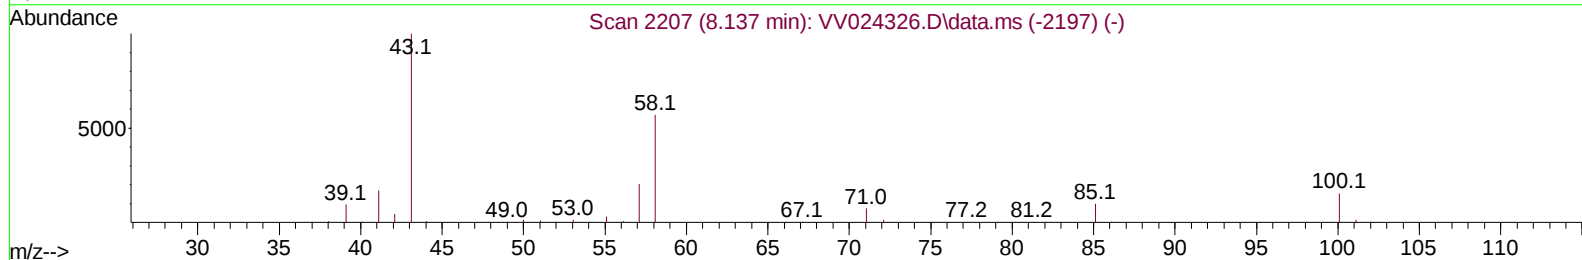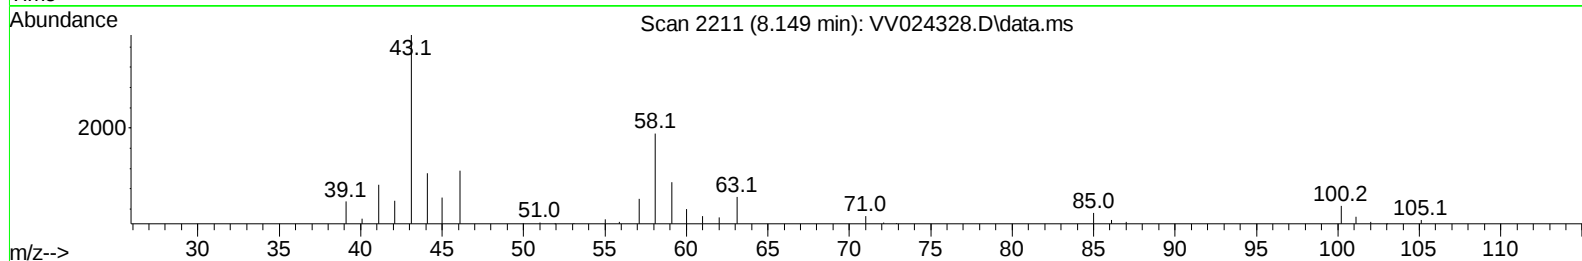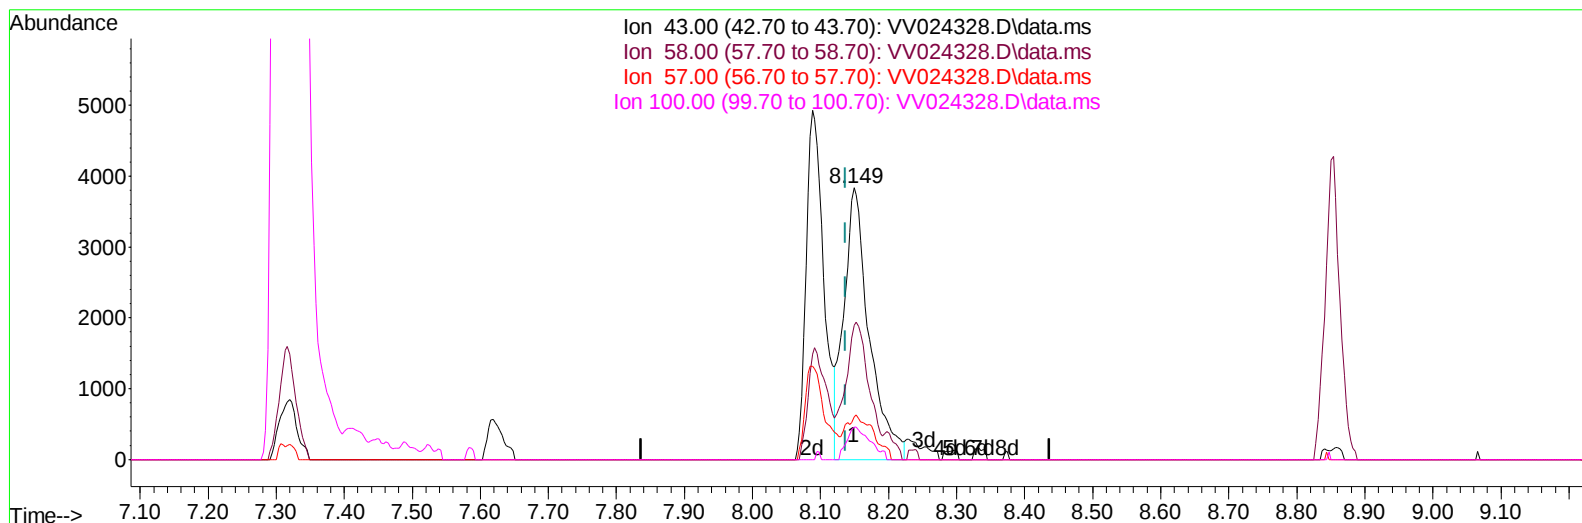

TIC: VV024328.D\data.ms

(48) 2-Hexanone (T)

8.149min (+ 0.013) 6.26 ug/L m

response 9908

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	56.20	44.82#
57.00	21.10	1.93#
100.00	16.20	10.54#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
 Data File : VV024328.D
 Acq On : 12 Jan 2022 12:58
 Operator : SY/MD
 Sample : VV0112WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK291

Manual IntegrationsAPPROVED

Quant Time: Jan 13 03:28:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	265691	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	252756	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	125822	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	91565	47.886	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	95.780%	
7) Chloroethane-d5	1.571	69	73478	50.585	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	101.160%	
11) 1,1-Dichloroethene-d2	2.111	63	139309	38.981	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	77.960%	
21) 2-Butanone-d5	3.895	46	104531	98.120	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	98.120%	
24) Chloroform-d	4.352	84	178546	51.090	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.180%	
26) 1,2-Dichloroethane-d4	5.034	65	120438	51.473	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.940%	
32) Benzene-d6	5.053	84	349909	53.050	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.100%	
36) 1,2-Dichloropropane-d6	6.069	67	100548	54.394	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	108.780%	
41) Toluene-d8	7.317	98	328310	51.409	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	102.820%	
43) trans-1,3-Dichloroprop...	7.622	79	53000	49.792	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	99.580%	
47) 2-Hexanone-d5	8.088	63	72977	90.869	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	90.870%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	125701	47.584	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	95.160%	
66) 1,2-Dichlorobenzene-d4	11.625	152	141442	56.398	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	112.800%	
Target Compounds						Qvalue
48) 2-Hexanone	8.149	43	9908m	6.258	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
Data File : VV024328.D
Acq On : 12 Jan 2022 12:58
Operator : SY/MD
Sample : VV0112WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK291

Manual IntegrationsAPPROVED

Quant Time: Jan 13 03:28:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

