




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
Data File : VV024340.D
Acq On : 12 Jan 2022 19:10
Operator : SY/MD
Sample : N1084-09 20X
Misc : 6.39g/5.0mL/100ul/5.0ml/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLN2

Manual IntegrationsAPPROVED

Quant Time: Jan 13 02:34:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/13/2022
Supervised By :Semsettin Yesilyurt 01/13/2022

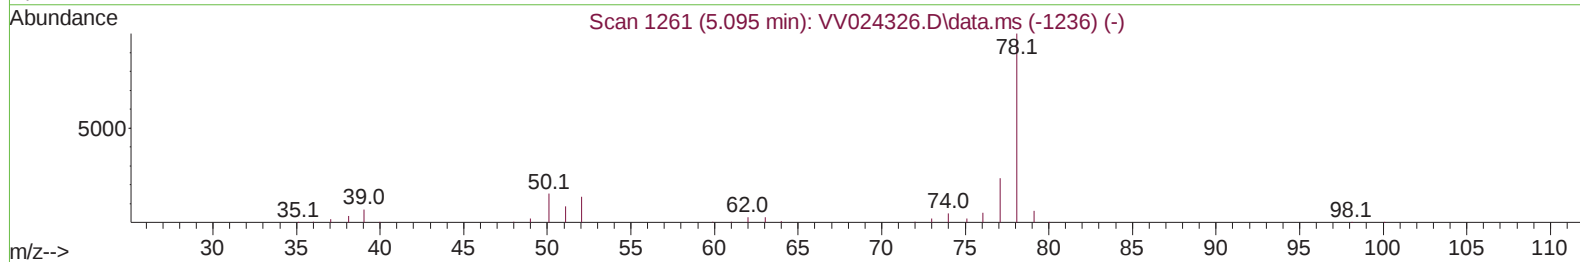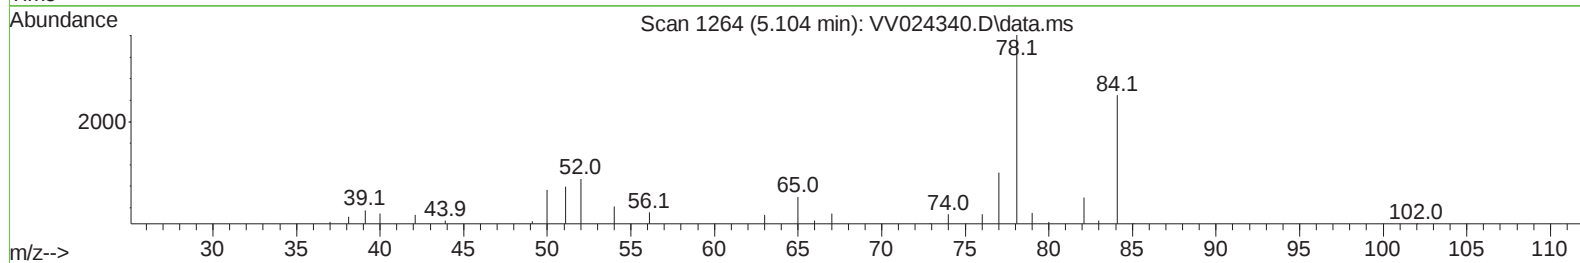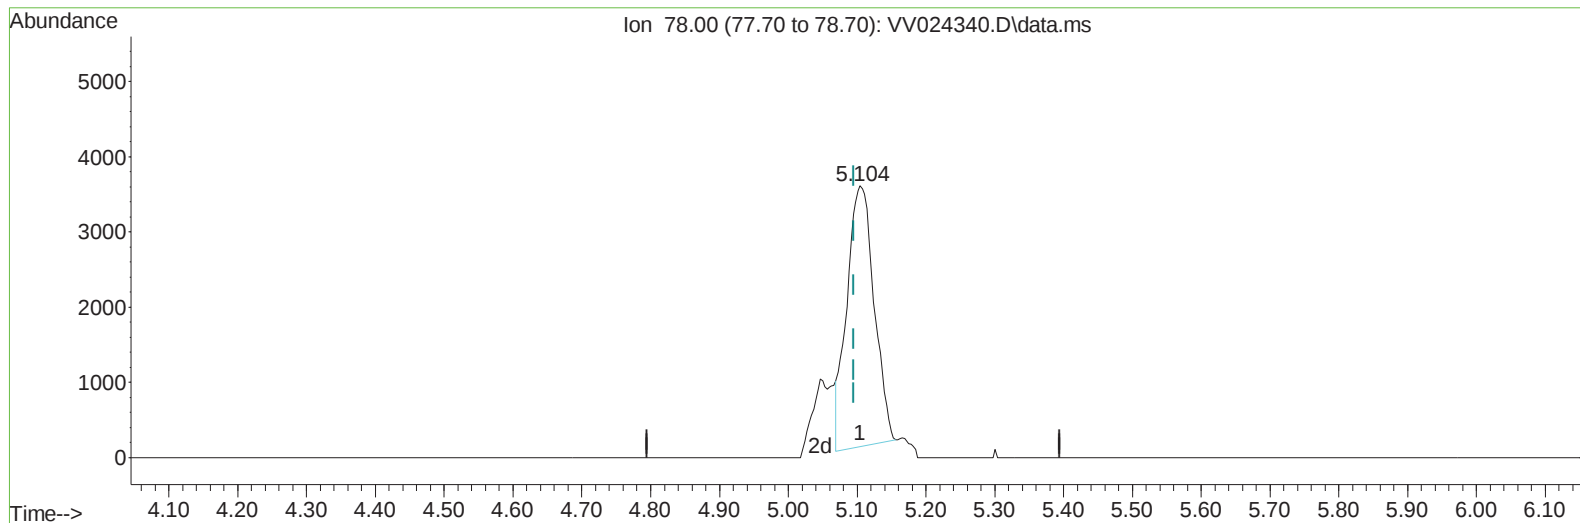

TIC: VV024340.D\data.ms

(33) Benzene (T)

5.104min (+ 0.010) 1.48 ug/L

response 9500

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
Data File : VV024340.D
Acq On : 12 Jan 2022 19:10
Operator : SY/MD
Sample : N1084-09 20X
Misc : 6.39g/5.0mL/100ul/5.0ml/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLN2

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
Supervised By :Semsettin Yesilyurt 01/13/2022

Quant Time: Jan 13 02:34:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

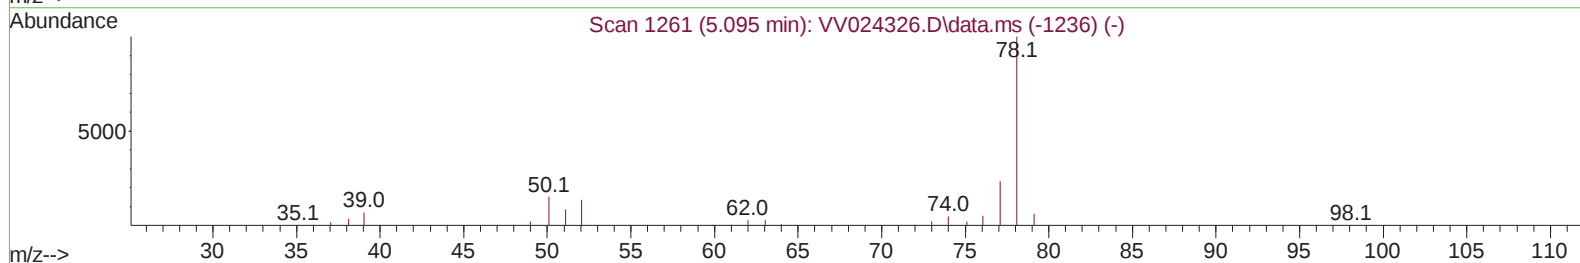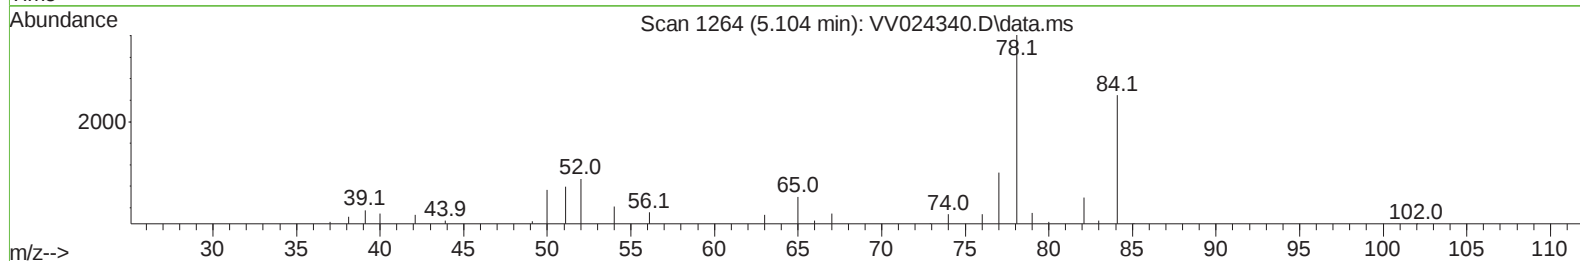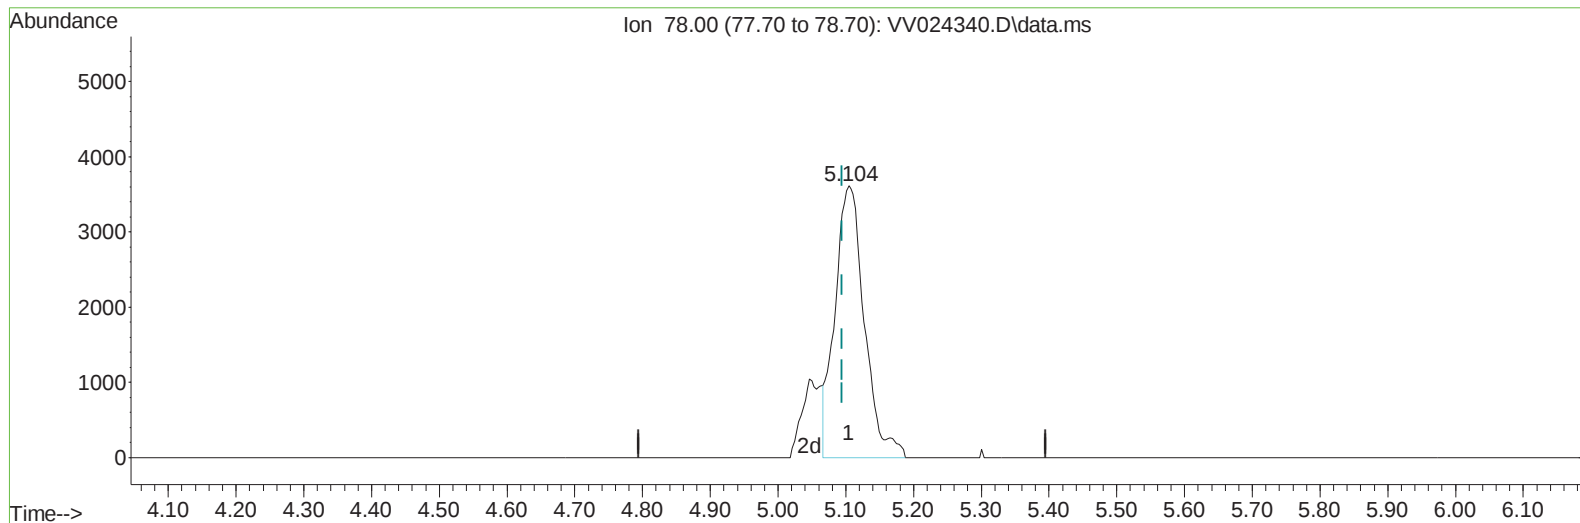

TIC: VV024340.D\data.ms

(33) Benzene (T)

5.104min (+ 0.010) 1.70 ug/L m

response 10880

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
Data File : VV024340.D
Acq On : 12 Jan 2022 19:10
Operator : SY/MD
Sample : N1084-09 20X
Misc : 6.39g/5.0mL/100ul/5.0ml/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLN2

Manual IntegrationsAPPROVED

Quant Time: Jan 13 02:34:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/13/2022
Supervised By :Semsettin Yesilyurt 01/13/2022

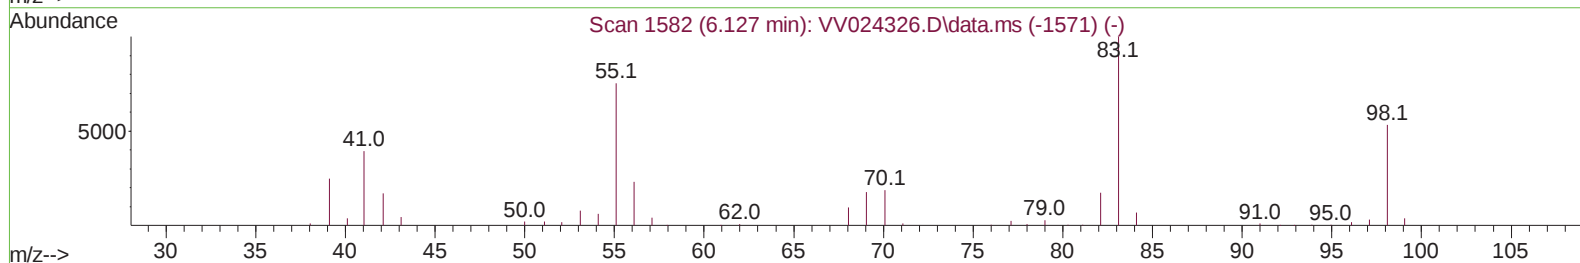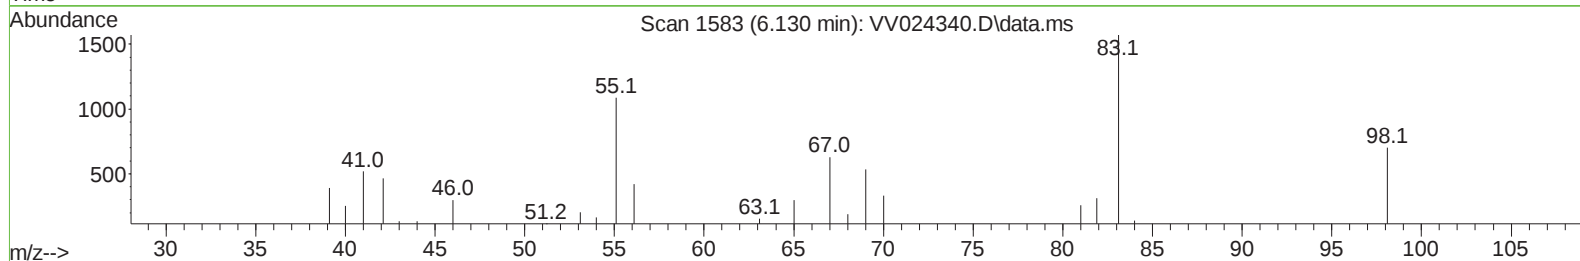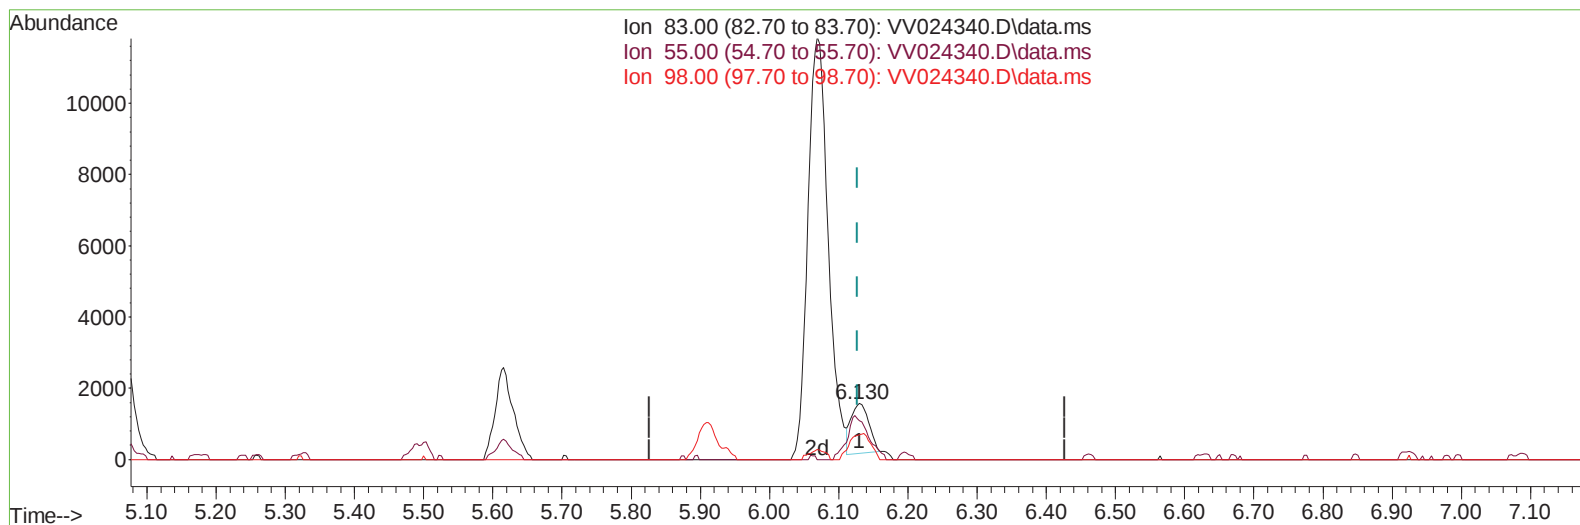

TIC: VV024340.D\data.ms

(35) Methylcyclohexane (T)

6.130min (+ 0.003) 0.95 ug/L

response 2491

Ion	Exp%	Act%
83.00	100.00	100.00
55.00	69.50	105.34#
98.00	51.60	62.10#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
Data File : VV024340.D
Acq On : 12 Jan 2022 19:10
Operator : SY/MD
Sample : N1084-09 20X
Misc : 6.39g/5.0mL/100ul/5.0ml/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLN2

Manual IntegrationsAPPROVED

Quant Time: Jan 13 02:34:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/13/2022
Supervised By :Semsettin Yesilyurt 01/13/2022

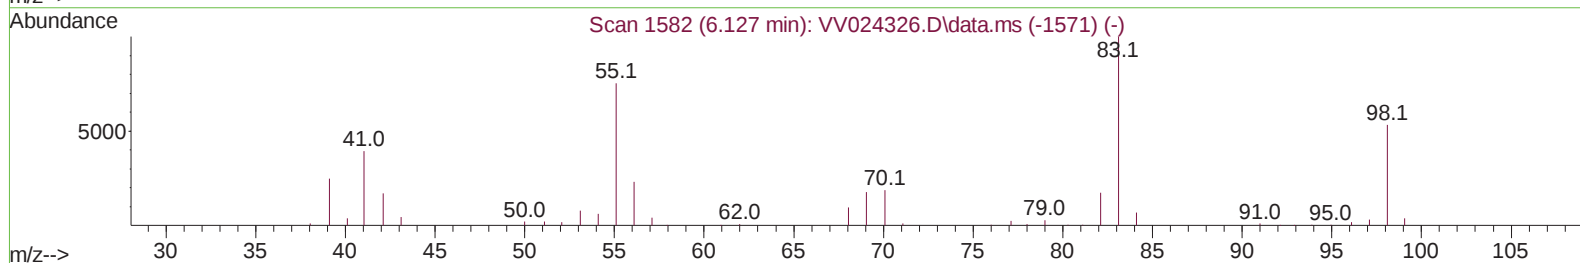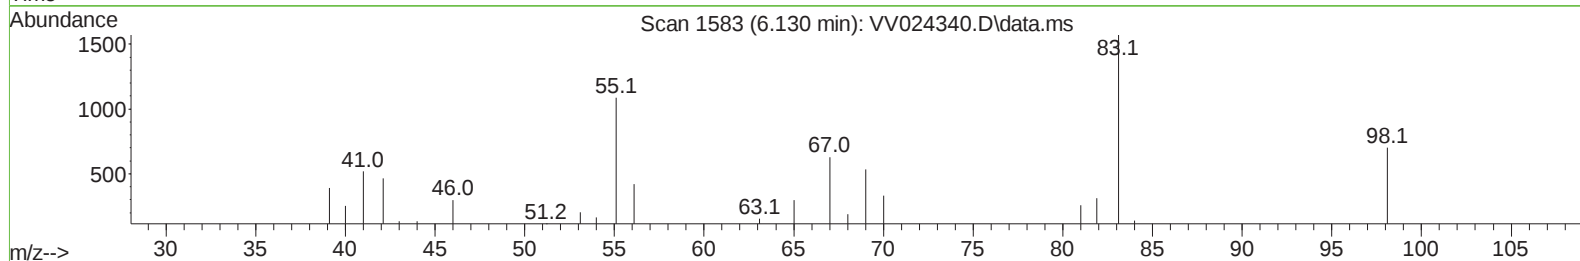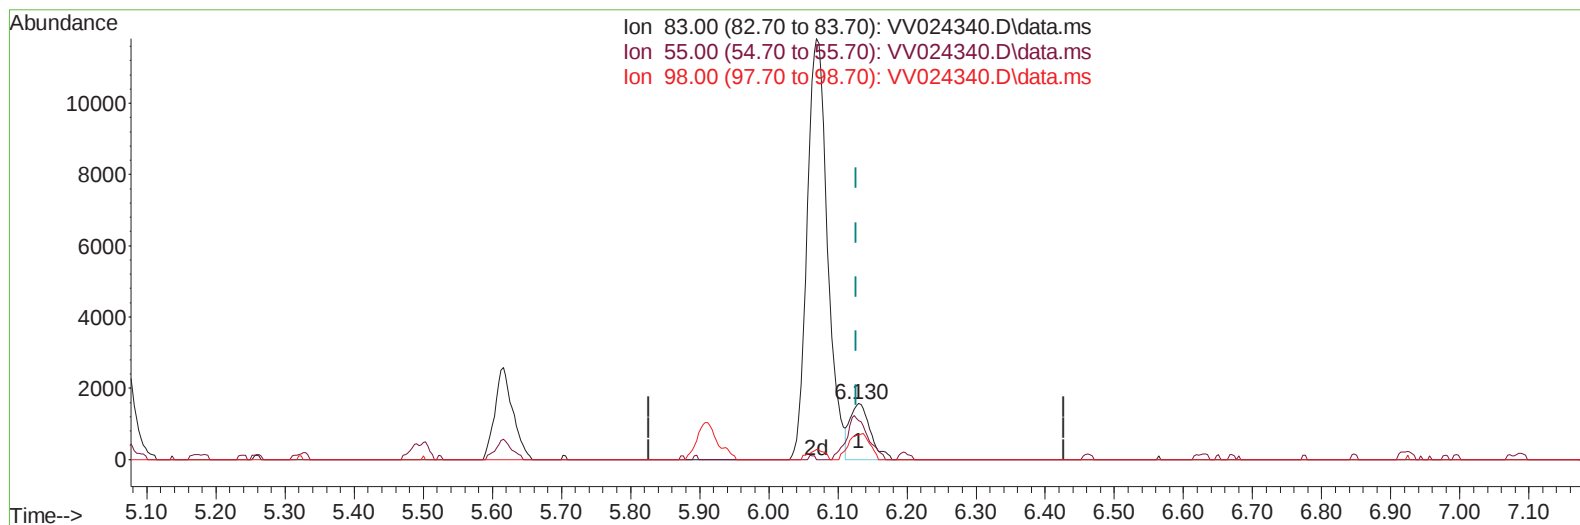

TIC: VV024340.D\data.ms

(35) Methylcyclohexane (T)

6.130min (+ 0.003) 1.23 ug/L m

response 3213

Ion	Exp%	Act%
83.00	100.00	100.00
55.00	69.50	81.67
98.00	51.60	48.15
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
 Data File : VV024340.D
 Acq On : 12 Jan 2022 19:10
 Operator : SY/MD
 Sample : N1084-09 20X
 Misc : 6.39g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLN2

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
 Supervised By :Semsettin Yesilyurt 01/13/2022

Quant Time: Jan 13 02:34:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	255755	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	251725	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	141426	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	81787	44.434	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	88.860%	
7) Chloroethane-d5	1.571	69	63958	45.741	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	91.480%	
11) 1,1-Dichloroethene-d2	2.108	63	122408	35.583	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.160%	
21) 2-Butanone-d5	3.889	46	97213	94.796	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	94.800%	
24) Chloroform-d	4.349	84	158104	46.998	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.000%	
26) 1,2-Dichloroethane-d4	5.030	65	107286	47.634	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.260%	
32) Benzene-d6	5.050	84	315283	47.996	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.000%	
36) 1,2-Dichloropropane-d6	6.069	67	91762	49.844	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	99.680%	
41) Toluene-d8	7.317	98	296241	46.577	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	93.160%	
43) trans-1,3-Dichloroprop...	7.622	79	47347	44.663	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.320%	
47) 2-Hexanone-d5	8.088	63	76545	95.702	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	95.700%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	131237	49.883	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	99.760%	
66) 1,2-Dichlorobenzene-d4	11.622	152	138358	49.081	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.160%	
Target Compounds						
						Qvalue
33) Benzene	5.104	78	10880m	1.700	ug/L	
35) Methylcyclohexane	6.130	83	3213m	1.227	ug/L	
42) Toluene	7.391	91	28649	3.987	ug/L	98
52) Ethylbenzene	9.011	91	600558	78.240	ug/L	100
53) m,p-Xylene	9.136	106	901657	293.056	ug/L	99
54) o-Xylene	9.542	106	221991	75.584	ug/L	97
60) Isopropylbenzene	9.931	105	66145	8.452	ug/L	99
62) 1,3,5-Trimethylbenzene	10.538	105	523859	77.819	ug/L	100
63) 1,2,4-Trimethylbenzene	10.914	105	1643560	244.558	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
Data File : VV024340.D
Acq On : 12 Jan 2022 19:10
Operator : SY/MD
Sample : N1084-09ME 20X
Misc : 6.39g/5.0mL/100ul/5.0ml/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLN2

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
Supervised By :Semsettin Yesilyurt 01/13/2022

Quant Time: Jan 13 02:34:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

