

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011222\
 Data File : VW024335.D
 Acq On : 12 Jan 2022 17:12
 Operator : SY/MD
 Sample : N1053-12
 Misc : 5.0ml/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jan 13 02:33:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	254034	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	239865	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	122071	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	85321	46.668	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.340%
7) Chloroethane-d5	1.568	69	67052	48.279	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.560%
11) 1,1-Dichloroethene-d2	2.108	63	127796	37.401	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.800%
21) 2-Butanone-d5	3.886	46	98371	96.575	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.570%
24) Chloroform-d	4.349	84	167774	50.211	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.420%
26) 1,2-Dichloroethane-d4	5.030	65	110424	49.359	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.720%
32) Benzene-d6	5.050	84	325042	51.928	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.860%
36) 1,2-Dichloropropane-d6	6.069	67	94585	53.918	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.840%
41) Toluene-d8	7.316	98	305048	50.334	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.660%
43) trans-1,3-Dichloroprop...	7.622	79	48974	48.482	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.960%
47) 2-Hexanone-d5	8.088	63	68480	89.852	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.850%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	116302	46.392	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.780%
66) 1,2-Dichlorobenzene-d4	11.622	152	128017	52.613	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.220%
Target Compounds						
					Qvalue	
48) 2-Hexanone	8.146	43	9243	6.152	ug/L	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
Data File : VV024335.D
Acq On : 12 Jan 2022 17:12
Operator : SY/MD
Sample : N1053-12
Misc : 5.0ml/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jan 13 02:33:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

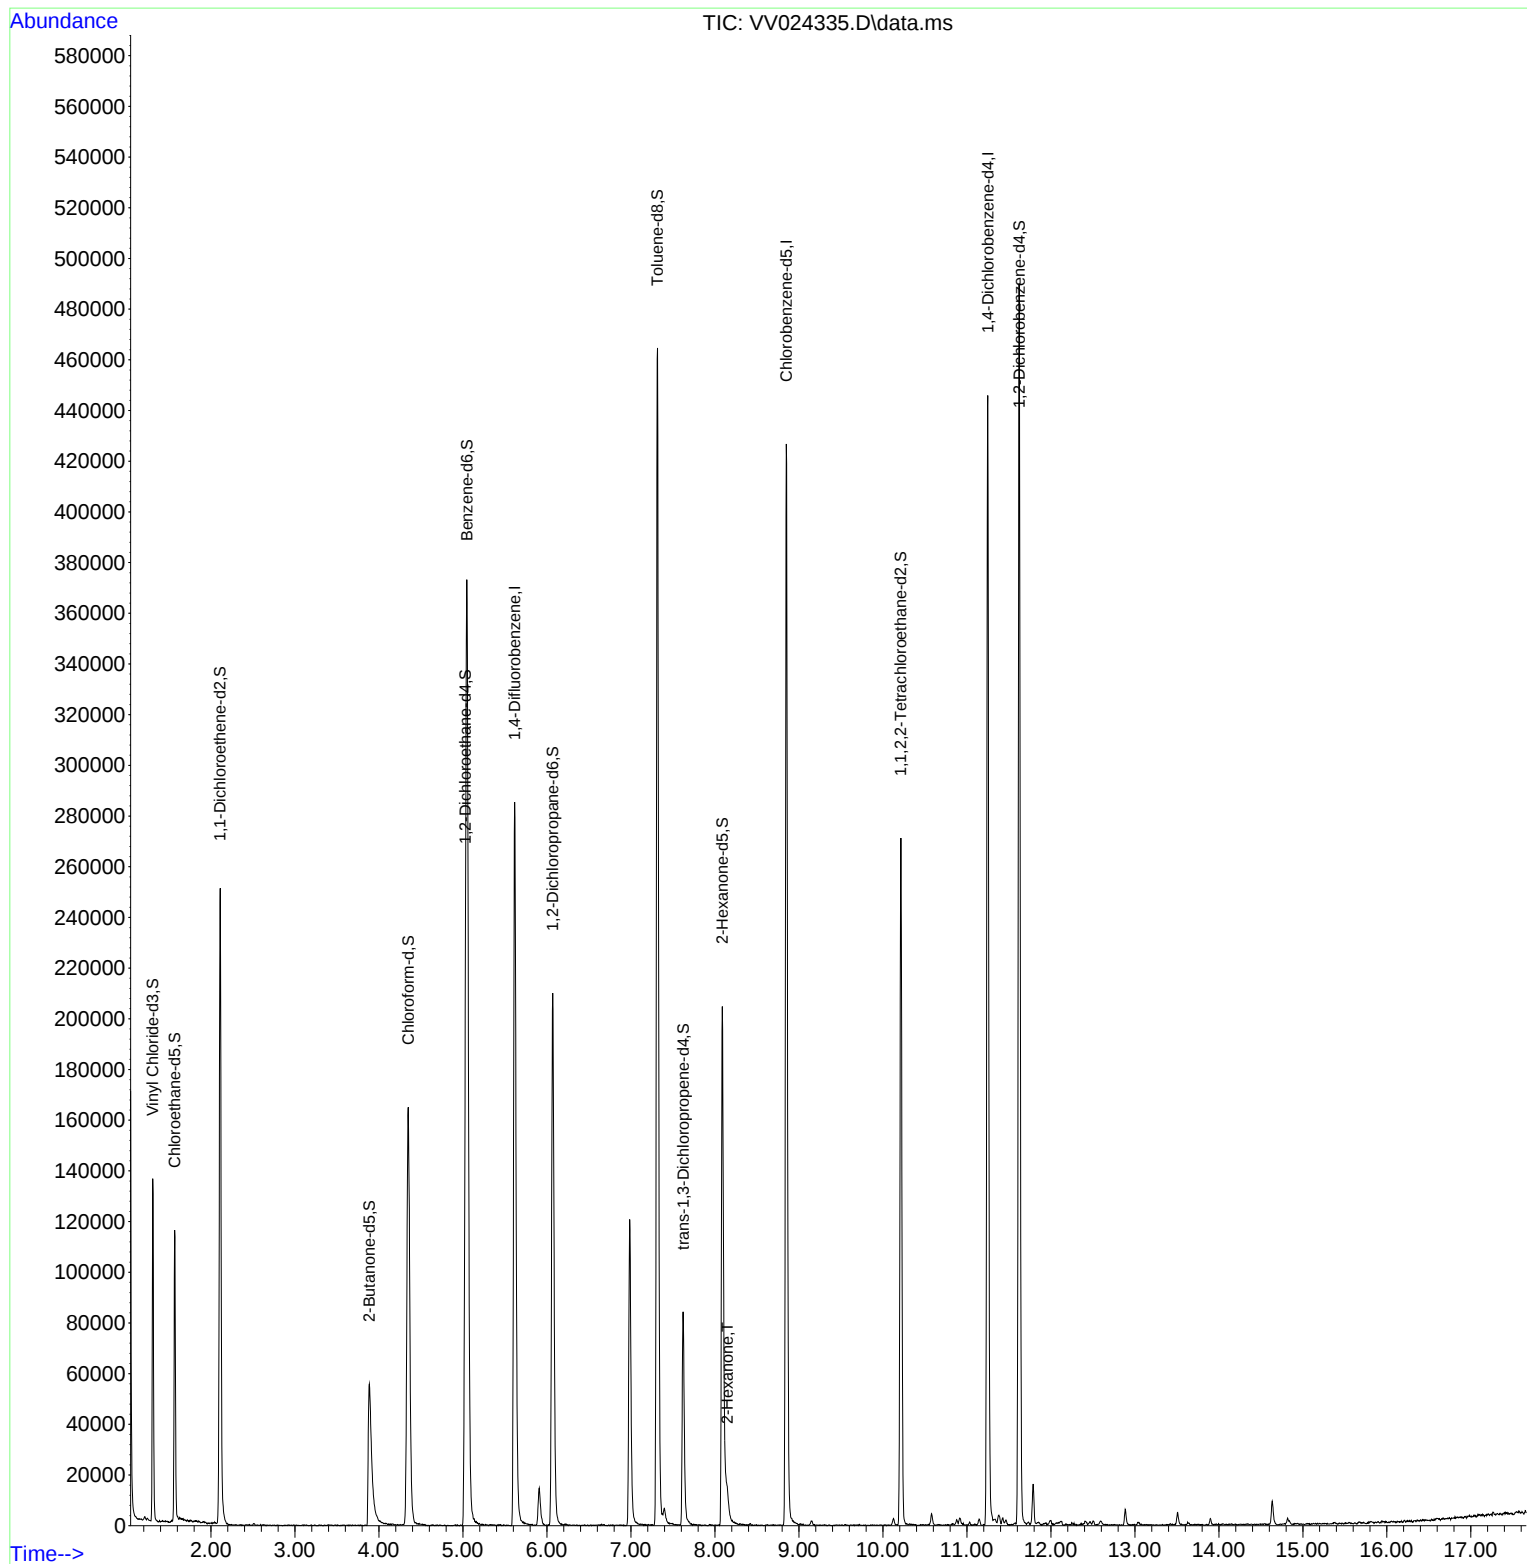

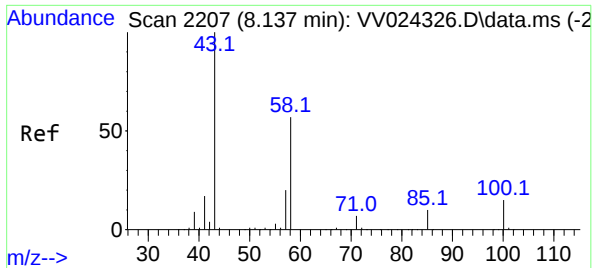

#48
 2-Hexanone
 Concen: 6.152 ug/L
 RT: 8.146 min Scan# 21
 Delta R.T. 0.009 min
 Lab File: VV024335.D
 Acq: 12 Jan 2022 17:12

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 43	Resp: 9243
Ion Ratio	Lower Upper
43 100	
58 53.4	45.0 67.4
57 16.4	16.9 25.3#
100 8.5	13.0 19.4#

