
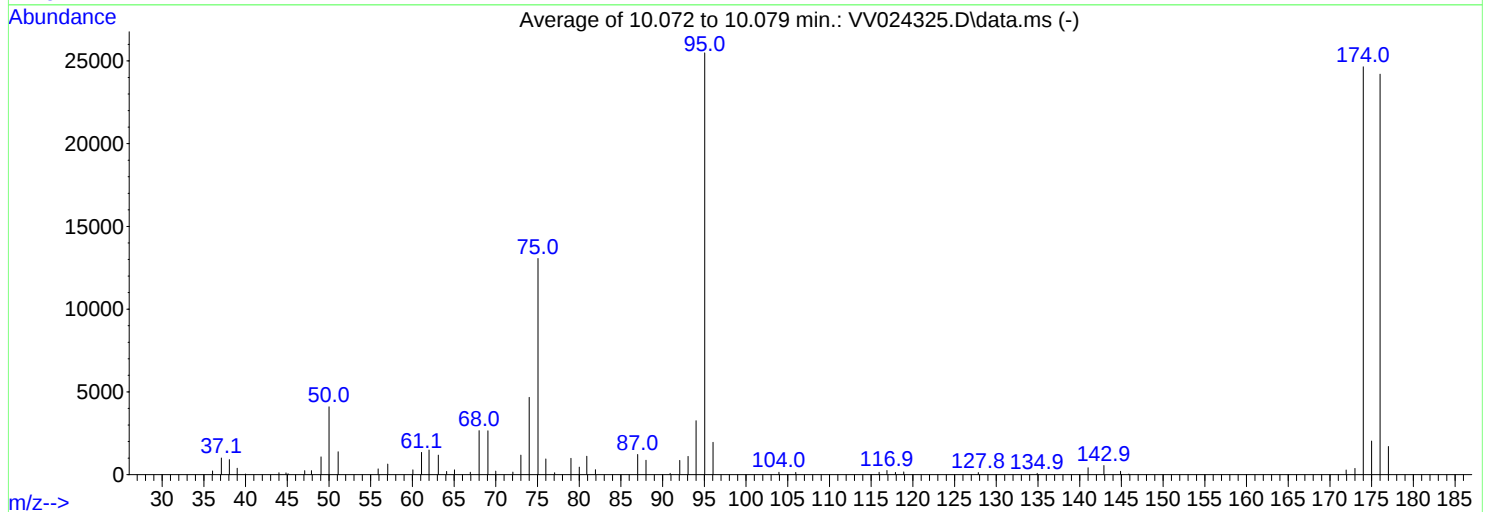


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011222\
 Data File : VV024325.D
 Acq On : 12 Jan 2022 11:32
 Operator : SY/MD
 Sample : BFB253
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB253

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis
 Last Update : Thu Jan 13 02:28:22 2022

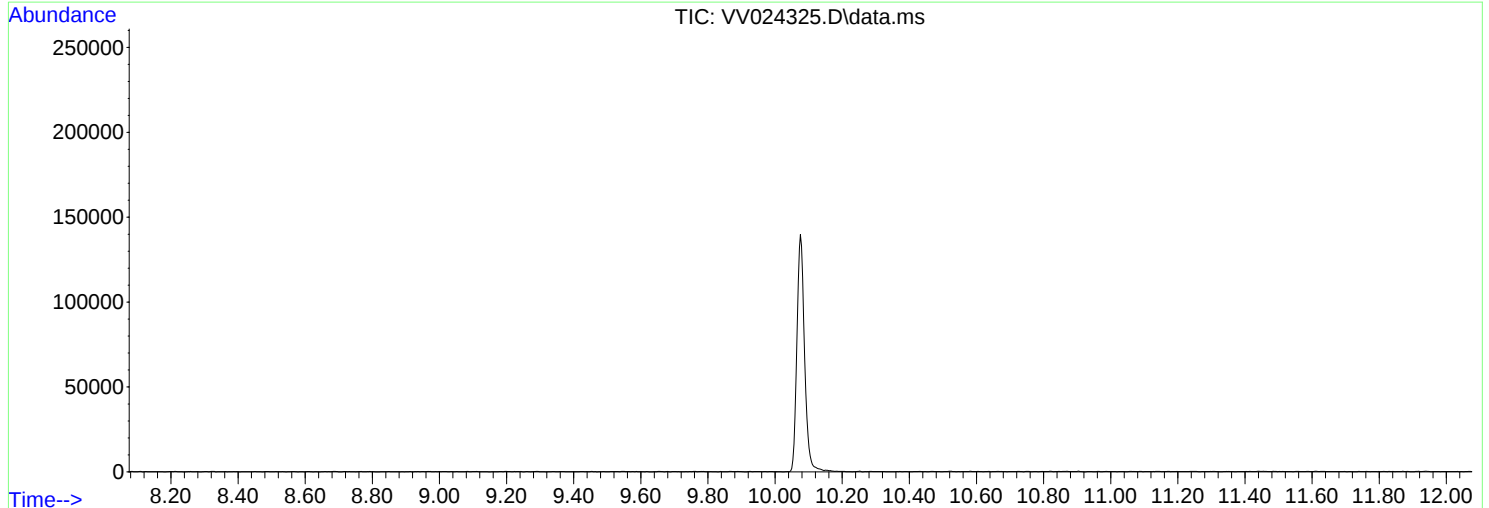

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	4099	PASS
75	95	30	80	51.2	13058	PASS
95	95	100	100	100.0	25488	PASS
96	95	5	9	7.7	1954	PASS
173	174	0.00	2	1.5	381	PASS
174	95	50	120	96.7	24643	PASS
175	174	5	9	8.2	2029	PASS
176	174	95	105	98.2	24203	PASS
177	176	5	10	7.0	1703	PASS

m/z	Abundance
44.00	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
36.00	218.0
37.10	1066.0
38.00	844.0
39.00	443.0
40.00	105.0
44.00	227.0
44.80	169.0
47.10	219.0
47.90	235.0
49.10	1074.0
50.00	4065.0
51.10	1407.0
55.90	338.0
57.00	655.0
60.10	343.0
61.10	1231.0
62.00	1486.0
63.10	1234.0
64.10	211.0
65.00	283.0
66.90	135.0
68.00	2605.0
69.00	2477.0
70.00	201.0
72.00	158.0
73.00	1159.0
74.00	4684.0
75.00	12732.0
76.00	898.0
77.00	106.0
79.00	929.0
80.00	406.0
80.90	1127.0
82.00	321.0
87.00	1127.0
88.00	943.0
90.90	122.0
92.10	873.0
93.10	1038.0
94.00	3195.0
95.00	25480.0
96.00	1980.0
104.00	120.0
106.00	140.0
116.00	156.0
116.90	260.0
117.90	155.0
118.90	137.0
127.80	119.0
141.00	435.0
142.90	510.0
144.90	221.0
171.90	238.0
173.00	353.0
174.00	23584.0
175.00	1961.0
176.00	23256.0
177.00	1682.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
36.10	229.0
37.10	1030.0
38.00	924.0
39.00	392.0
44.00	255.0
44.90	154.0
47.10	249.0
47.90	250.0
49.10	1118.0
50.00	4219.0
51.10	1442.0
55.90	356.0
57.00	649.0
60.10	296.0
61.10	1393.0
62.00	1516.0
63.10	1199.0
64.10	203.0
65.10	311.0
67.00	158.0
68.00	2741.0
69.00	2762.0
70.00	223.0
72.00	169.0
73.00	1245.0
74.00	4792.0
75.10	13560.0
76.00	942.0
77.10	126.0
79.00	1040.0
80.00	497.0
80.90	1126.0
82.00	293.0
87.00	1338.0
88.00	868.0
90.90	102.0
92.10	908.0
93.10	1112.0
94.00	3436.0
95.00	26496.0
96.10	2106.0
103.90	154.0
106.00	134.0
115.90	144.0
116.90	271.0
117.90	148.0
118.90	163.0
127.80	131.0
134.90	115.0
141.00	443.0
142.90	576.0
144.90	202.0
145.90	105.0
171.90	277.0
173.00	387.0
174.00	25416.0
175.00	2123.0
176.00	24984.0
177.00	1730.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
36.00	222.0
37.10	909.0
38.10	948.0
39.00	320.0
44.00	291.0
45.10	169.0
47.10	255.0
47.90	235.0
49.00	1034.0
50.00	4013.0
51.10	1301.0
55.90	339.0
57.10	615.0
60.00	230.0
61.10	1395.0
62.00	1478.0
63.10	1111.0
64.10	181.0
65.10	266.0
67.00	157.0
68.00	2640.0
69.10	2702.0
70.00	210.0
72.10	133.0
73.00	1132.0
74.00	4541.0
75.10	12882.0
76.00	995.0
77.10	132.0
79.00	995.0
80.00	446.0
80.90	1071.0
81.90	276.0
87.00	1186.0
88.00	804.0
92.00	796.0
93.00	1155.0
94.00	3156.0
95.10	24488.0
96.10	1775.0
103.90	158.0
105.90	128.0
115.90	126.0
116.90	238.0
117.90	112.0
118.90	187.0
127.90	130.0
134.90	115.0
141.00	368.0
142.90	581.0
144.90	194.0
172.00	330.0
173.00	402.0
174.00	24928.0
175.00	2004.0
176.00	24368.0
177.00	1696.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253