
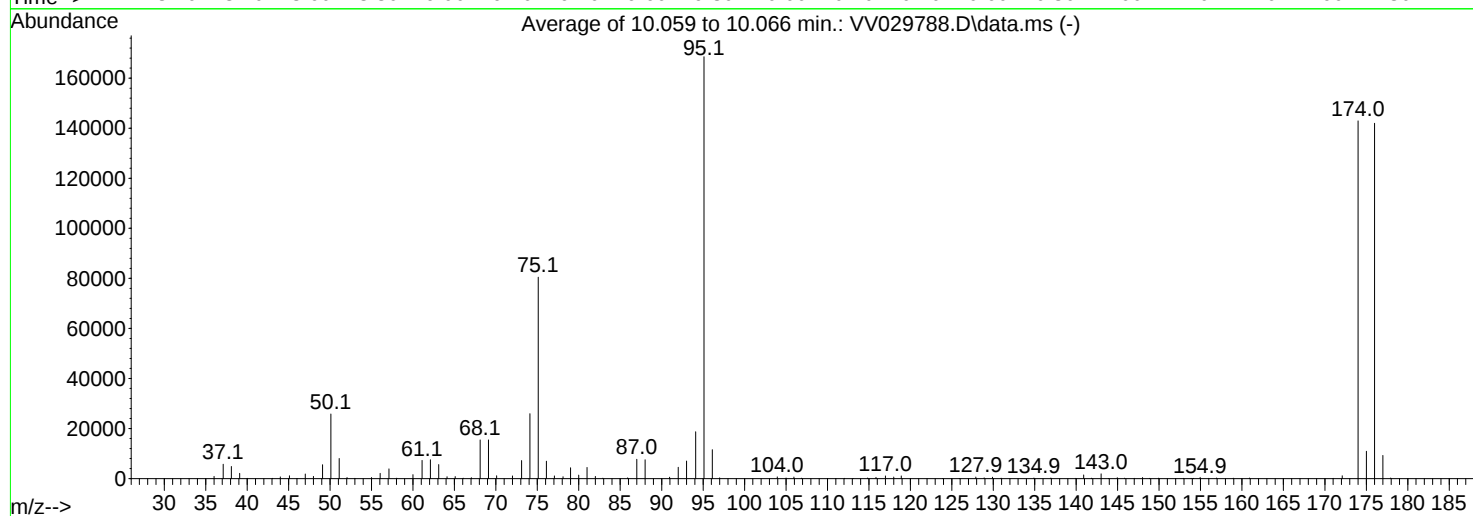


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011223\
Data File : VV029788.D
Acq On : 12 Jan 2023 15:56
Operator : SY/MD
Sample : BFB211
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB211

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 12 22:05:54 2023

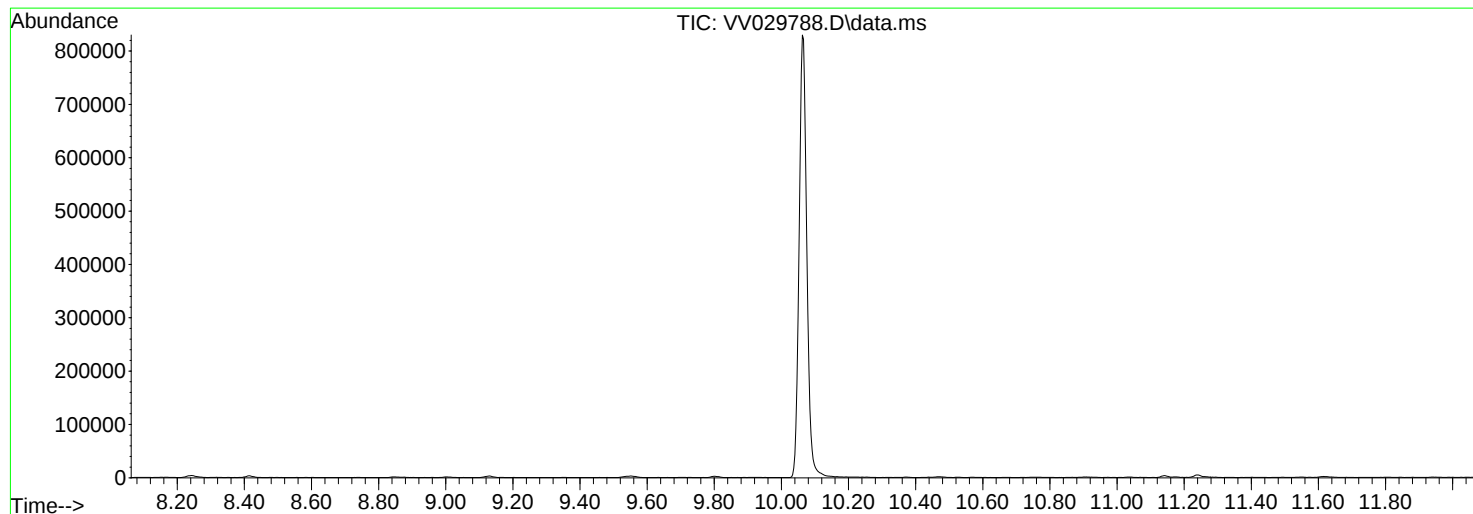

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	25811	PASS
75	95	30	80	47.8	80501	PASS
95	95	100	100	100.0	168555	PASS
96	95	5	9	6.9	11568	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.8	142912	PASS
175	174	5	9	7.6	10917	PASS
176	174	95	105	99.4	141995	PASS
177	176	5	10	6.5	9241	PASS

m/z	Abundance
40.00	111.0
44.00	460.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	863.0
37.10	5560.0
38.10	4815.0
39.10	2043.0
40.00	208.0
43.00	117.0
44.00	1115.0
45.10	1038.0
47.00	1667.0
48.00	857.0
49.10	5279.0
50.10	24672.0
51.10	7779.0
52.00	402.0
53.00	115.0
55.00	392.0
56.10	2131.0
57.10	3528.0
58.00	172.0
60.00	1527.0
61.10	6996.0
62.10	7089.0
63.10	5201.0
64.10	732.0
65.10	744.0
66.00	145.0
67.00	313.0
68.10	14816.0
69.10	14860.0
70.10	1086.0
72.00	1011.0
73.10	7070.0
74.10	24744.0
75.10	76848.0
76.10	6569.0
77.10	1037.0
78.10	735.0
79.00	4224.0
80.00	1337.0
81.00	4217.0
82.00	834.0
82.90	112.0
85.90	260.0
87.00	7348.0
88.00	7089.0
91.00	558.0
92.00	4284.0
93.00	6536.0
94.10	17680.0
95.10	159488.0
96.10	10883.0
97.00	333.0
103.90	671.0
105.00	260.0
105.90	564.0
106.80	108.0
112.10	110.0
113.10	109.0
114.90	203.0
115.80	428.0
117.00	970.0
118.00	583.0
118.90	1032.0
123.90	101.0
127.90	605.0
128.90	307.0
129.90	536.0
131.00	177.0
134.90	253.0
137.00	210.0
140.90	1261.0
141.90	157.0
143.00	1785.0
144.90	292.0
145.80	150.0
147.00	107.0
148.00	394.0
148.90	114.0
149.90	154.0
153.00	130.0
153.90	135.0
155.00	361.0
157.00	192.0
159.00	171.0
160.90	222.0
172.10	995.0
174.00	132160.0
175.00	10311.0
176.00	132800.0
177.00	8717.0
177.90	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	929.0
37.10	5886.0
38.10	5025.0
39.10	2105.0
40.10	212.0
44.10	1140.0
45.10	1160.0
47.00	1880.0
48.00	875.0
49.10	5686.0
50.10	26664.0
51.10	8307.0
52.10	475.0
53.00	118.0
55.00	426.0
56.00	2192.0
57.10	4002.0
58.00	179.0
60.00	1598.0
61.10	7453.0
62.10	7900.0
63.10	5760.0
64.10	763.0
65.10	831.0
66.10	153.0
67.00	383.0
68.10	16017.0
69.10	15846.0
70.10	1153.0
72.00	1107.0
73.10	7496.0
74.10	26760.0
75.10	82984.0
76.10	7091.0
77.10	1114.0
78.10	768.0
79.00	4433.0
80.00	1436.0
81.00	4605.0
82.00	910.0
82.90	171.0
85.90	277.0
87.00	8037.0
88.00	7783.0
91.00	580.0
92.00	4661.0
93.00	7245.0
94.10	19232.0
95.10	174080.0
96.10	11998.0
97.00	311.0
104.00	719.0
105.00	246.0
106.00	659.0
106.90	139.0
110.00	108.0
112.10	133.0
114.90	221.0
115.80	508.0
117.00	1076.0
118.00	599.0
118.90	1110.0
125.90	111.0
127.90	613.0
128.90	298.0
129.90	558.0
130.90	168.0
134.90	256.0
137.00	207.0
139.90	122.0
140.90	1472.0
141.80	187.0
143.00	1922.0
143.90	103.0
145.00	367.0
145.90	164.0
147.00	103.0
148.00	429.0
148.90	118.0
149.90	201.0
153.00	125.0
154.10	126.0
155.00	480.0
156.00	102.0
157.00	238.0
159.00	194.0
160.90	269.0
171.00	152.0
172.10	1166.0
174.00	147968.0
175.00	11244.0
176.00	147200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

177.009575.0

178.00235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	856.0
37.10	5710.0
38.10	4722.0
39.10	2013.0
40.10	214.0
43.10	144.0
44.10	1120.0
45.10	1155.0
46.00	167.0
47.00	1939.0
48.00	802.0
49.10	5608.0
50.10	26096.0
51.10	8004.0
52.00	474.0
53.00	129.0
55.00	442.0
56.00	1982.0
57.10	4087.0
58.10	158.0
60.00	1543.0
61.10	7272.0
62.10	7656.0
63.10	5747.0
64.10	702.0
65.10	888.0
66.10	145.0
67.10	412.0
68.10	15564.0
69.10	15609.0
70.10	1087.0
72.00	1027.0
73.10	7005.0
74.10	26296.0
75.10	81672.0
76.10	7095.0
77.00	1100.0
78.10	767.0
79.00	4240.0
80.00	1429.0
81.00	4606.0
82.00	914.0
82.90	176.0
85.90	290.0
87.00	7828.0
88.00	7666.0
90.90	580.0
92.00	4572.0
93.00	7176.0
94.10	19128.0
95.10	172096.0
96.10	11824.0
97.00	296.0
104.00	725.0
105.00	216.0
106.00	709.0
106.90	170.0
110.00	101.0
111.00	108.0
112.00	130.0
114.80	187.0
115.90	561.0
117.00	1094.0
118.00	599.0
118.90	962.0
127.90	578.0
128.90	252.0
129.90	527.0
130.90	188.0
134.90	245.0
136.90	203.0
140.00	140.0
140.90	1522.0
141.80	202.0
143.00	1917.0
145.00	419.0
145.90	183.0
147.00	108.0
148.00	440.0
148.80	136.0
150.00	241.0
152.00	117.0
152.90	124.0
153.80	108.0
154.20	110.0
154.90	593.0
156.00	116.0
156.90	229.0
158.90	207.0
160.90	293.0
171.00	178.0
172.10	1254.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

174.00	148608.0
175.00	11197.0
176.00	145984.0
177.00	9432.0
178.00	262.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211