


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011320\
Data File : VV014275.D
Acq On : 13 Jan 2020 09:06
Operator : SY/MD
Sample : BFB54
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB54

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jan 11 00:01:14 2020

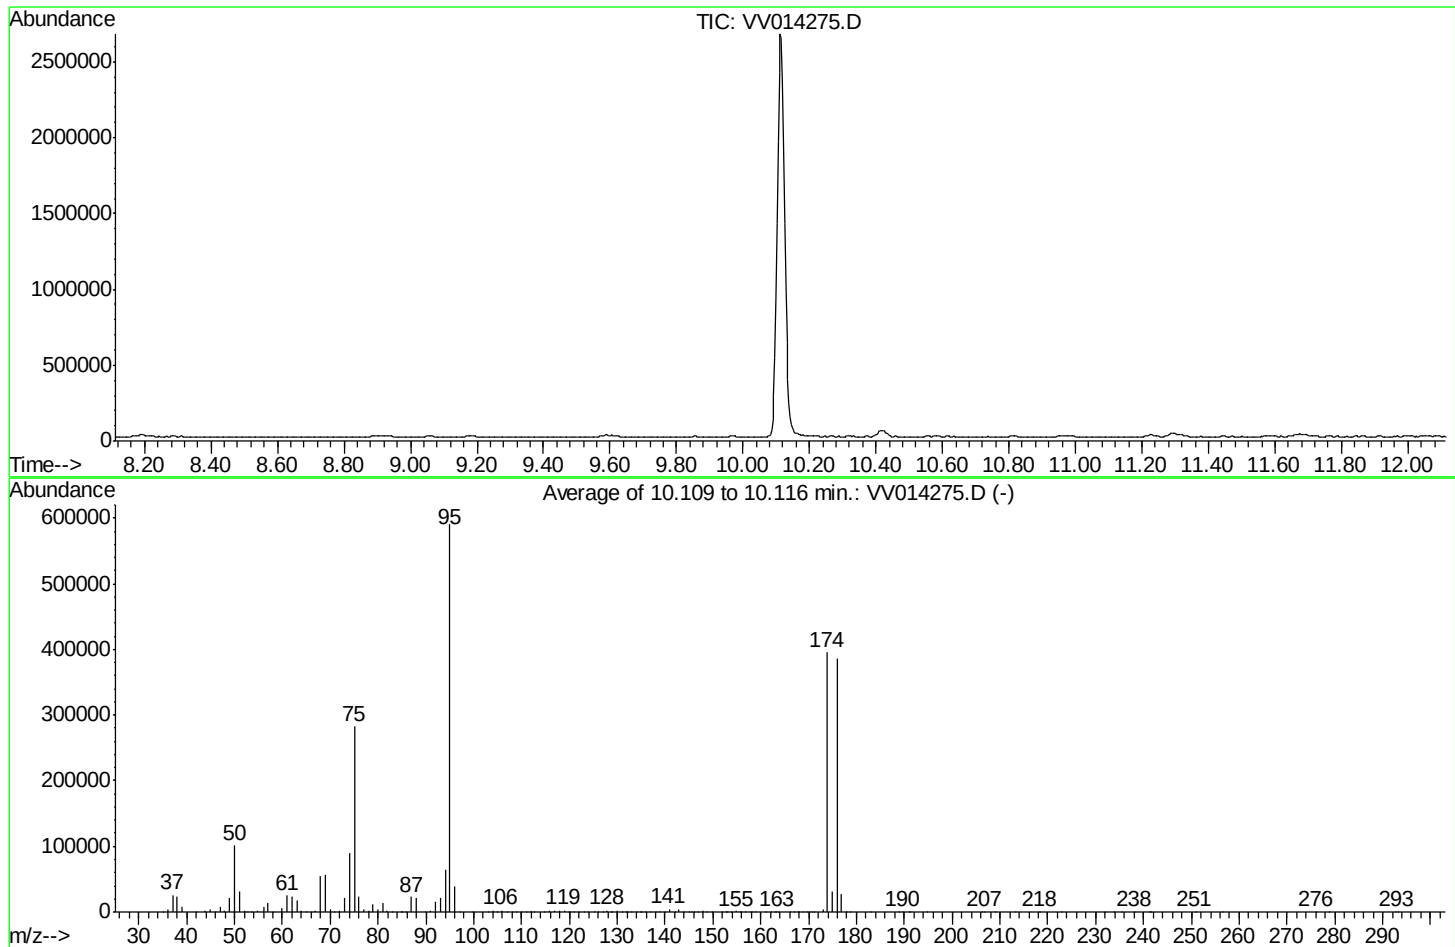

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	100840	PASS
75	95	30	80	47.8	282563	PASS
95	95	100	100	100.0	590635	PASS
96	95	5	9	6.5	38150	PASS
173	174	0.00	2	1.1	4475	PASS
174	95	50	120	66.9	395008	PASS
175	174	5	9	7.8	30952	PASS
176	174	95	101	97.6	385642	PASS
177	176	5	9	6.9	26427	PASS