

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011321\
 Data File : VV019979.D
 Acq On : 13 Jan 2021 11:03
 Operator : SY/MD
 Sample : VV0113WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV019979.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	250429	244776	15.03%	1.933%
2	1.569	142	149	160	rBV	204730	229526	14.10%	1.812%
3	2.110	307	317	349	rVB	430367	659869	40.53%	5.210%
4	2.515	435	443	449	rBV4	2870	4460	0.27%	0.035%
5	2.704	500	502	505	rVB4	606	316	0.02%	0.002%
6	2.765	518	521	524	rBV3	826	641	0.04%	0.005%
7	2.881	553	557	560	rBV2	561	349	0.02%	0.003%
8	2.910	560	566	571	rBV5	899	642	0.04%	0.005%
9	2.939	572	575	577	rBV2	682	364	0.02%	0.003%
10	2.984	587	589	592	rBV2	630	373	0.02%	0.003%
11	3.032	602	604	609	rVB3	564	310	0.02%	0.002%
12	3.344	698	701	704	rBV3	510	467	0.03%	0.004%
13	3.534	757	760	762	rBV	645	324	0.02%	0.003%
14	3.556	765	767	771	rVB4	681	347	0.02%	0.003%
15	3.598	777	780	783	rVB3	930	568	0.03%	0.004%
16	3.614	783	785	787	rBV	702	454	0.03%	0.004%
17	3.682	802	806	809	rBV2	464	310	0.02%	0.002%
18	3.720	813	818	820	rBV3	802	560	0.03%	0.004%
19	3.897	861	873	912	rBV	111864	360428	22.14%	2.846%
20	4.354	999	1015	1042	rBV	275049	677302	41.60%	5.348%
21	4.589	1086	1088	1091	rBV3	603	312	0.02%	0.002%
22	4.916	1187	1190	1192	rBV2	613	295	0.02%	0.002%
23	4.933	1192	1195	1199	rVB4	687	576	0.04%	0.005%
24	4.981	1207	1210	1214	rBV4	940	725	0.04%	0.006%
25	5.052	1214	1232	1258	rBV2	634821	1628214	100.00%	12.856%
26	5.431	1347	1350	1352	rBV3	907	626	0.04%	0.005%
27	5.473	1361	1363	1368	rBV5	869	697	0.04%	0.006%
28	5.621	1397	1409	1437	rBV	477572	966818	59.38%	7.634%
29	5.830	1472	1474	1476	rBV	563	327	0.02%	0.003%
30	5.910	1490	1499	1517	rVB3	30667	65759	4.04%	0.519%
31	5.990	1522	1524	1527	rBV4	681	302	0.02%	0.002%
32	6.074	1536	1550	1583	rBV	365145	752825	46.24%	5.944%
33	6.312	1621	1624	1627	rBV2	703	586	0.04%	0.005%
34	6.392	1643	1649	1652	rBV5	768	713	0.04%	0.006%
35	6.412	1652	1655	1657	rVV2	965	464	0.03%	0.004%
36	6.437	1661	1663	1666	rVV2	510	281	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011321\
 Data File : VV019979.D
 Acq On : 13 Jan 2021 11:03
 Operator : SY/MD
 Sample : VV0113WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.572	1703	1705	1708	rVB	846	366	0.02%	0.003%
38	6.797	1774	1775	1779	rBV4	613	380	0.02%	0.003%
39	6.817	1779	1781	1785	rVB3	852	467	0.03%	0.004%
40	6.910	1806	1810	1813	rBV4	626	490	0.03%	0.004%
41	6.990	1823	1835	1854	rBV	204359	369595	22.70%	2.918%
42	7.174	1888	1892	1894	rBV4	978	795	0.05%	0.006%
43	7.322	1925	1938	1964	rBV	726176	1256772	77.19%	9.924%
44	7.627	2022	2033	2050	rBV	141304	249937	15.35%	1.974%
45	7.913	2118	2122	2128	rBV4	680	655	0.04%	0.005%
46	7.984	2136	2144	2151	rVB9	2110	3443	0.21%	0.027%
47	8.048	2162	2164	2168	rBV2	439	289	0.02%	0.002%
48	8.093	2168	2178	2218	rBV2	377562	764906	46.98%	6.040%
49	8.421	2277	2280	2283	rBV3	819	659	0.04%	0.005%
50	8.447	2286	2288	2290	rBV2	852	460	0.03%	0.004%
51	8.614	2337	2340	2342	rBV4	734	479	0.03%	0.004%
52	8.672	2356	2358	2361	rVV2	496	300	0.02%	0.002%
53	8.730	2373	2376	2382	rBV7	966	893	0.05%	0.007%
54	8.756	2382	2384	2386	rVV2	833	399	0.02%	0.003%
55	8.768	2386	2388	2394	rVV6	565	411	0.03%	0.003%
56	8.858	2404	2416	2437	rBV	747748	1206637	74.11%	9.528%
57	9.022	2463	2467	2471	rBV5	1066	941	0.06%	0.007%
58	9.154	2503	2508	2510	rBV3	836	843	0.05%	0.007%
59	9.264	2539	2542	2545	rBV4	767	474	0.03%	0.004%
60	9.437	2593	2596	2599	rBV3	503	374	0.02%	0.003%
61	9.540	2626	2628	2629	rBV	691	312	0.02%	0.002%
62	9.563	2633	2635	2637	rVV3	839	531	0.03%	0.004%
63	9.588	2641	2643	2647	rVB4	962	472	0.03%	0.004%
64	9.756	2692	2695	2699	rBV3	636	553	0.03%	0.004%
65	9.778	2699	2702	2707	rVB3	891	884	0.05%	0.007%
66	9.807	2707	2711	2714	rBV3	827	611	0.04%	0.005%
67	9.891	2735	2737	2741	rBV4	430	338	0.02%	0.003%
68	9.981	2762	2765	2768	rBV3	950	729	0.04%	0.006%
69	10.013	2774	2775	2778	rBV	441	297	0.02%	0.002%
70	10.157	2818	2820	2824	rVB2	636	428	0.03%	0.003%
71	10.222	2828	2840	2860	rVV	460888	716884	44.03%	5.661%
72	10.357	2879	2882	2885	rBV2	579	412	0.03%	0.003%
73	10.402	2892	2896	2899	rBV4	722	650	0.04%	0.005%
74	10.476	2917	2919	2923	rVB3	761	420	0.03%	0.003%
75	10.546	2936	2941	2946	rBV6	899	851	0.05%	0.007%
76	10.588	2950	2954	2959	rVB4	969	919	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011321\
 Data File : VV019979.D
 Acq On : 13 Jan 2021 11:03
 Operator : SY/MD
 Sample : VV0113WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.614	2959	2962	2964	rBV	493	348	0.02%	0.003%
78	10.984	3075	3077	3082	rVB4	733	445	0.03%	0.004%
79	11.096	3110	3112	3117	rVV3	587	469	0.03%	0.004%
80	11.119	3117	3119	3124	rVB5	554	400	0.02%	0.003%
81	11.190	3138	3141	3143	rBV3	719	450	0.03%	0.004%
82	11.257	3149	3162	3188	rBV	784767	1227574	75.39%	9.693%
83	11.630	3266	3278	3298	rBV	796640	1236262	75.93%	9.762%
84	12.061	3410	3412	3415	rBV3	642	432	0.03%	0.003%
85	12.135	3431	3435	3440	rBV5	615	797	0.05%	0.006%
86	12.157	3440	3442	3444	rVB2	748	285	0.02%	0.002%
87	12.370	3506	3508	3511	rBV3	613	393	0.02%	0.003%
88	12.402	3516	3518	3520	rBV2	612	301	0.02%	0.002%
89	12.511	3549	3552	3555	rBV3	668	432	0.03%	0.003%
90	12.585	3571	3575	3577	rBV3	1002	862	0.05%	0.007%
91	12.627	3584	3588	3589	rBV3	700	442	0.03%	0.003%
92	12.929	3680	3682	3687	rVB3	936	706	0.04%	0.006%
93	12.961	3687	3692	3693	rBV2	645	480	0.03%	0.004%
94	13.051	3715	3720	3722	rBV3	777	620	0.04%	0.005%
95	13.273	3785	3789	3795	rBV7	1769	1919	0.12%	0.015%
96	13.357	3813	3815	3819	rBV3	658	470	0.03%	0.004%
97	13.617	3894	3896	3899	rBV2	742	470	0.03%	0.004%
98	13.961	4000	4003	4007	rBV3	1001	997	0.06%	0.008%
99	14.434	4147	4150	4151	rBV2	573	358	0.02%	0.003%
100	14.678	4223	4226	4227	rBV2	943	455	0.03%	0.004%




Sum of corrected areas: 12664529

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011321\
Data File : VV019979.D
Acq On : 13 Jan 2021 11:03
Operator : SY/MD
Sample : VV0113WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK73

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

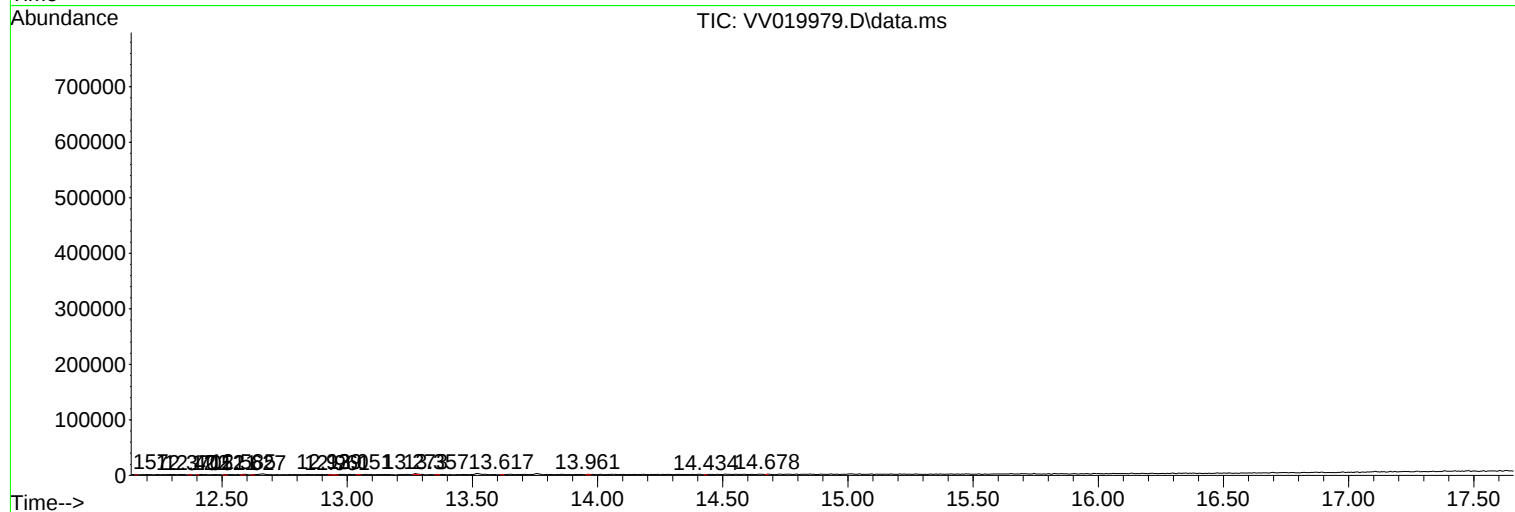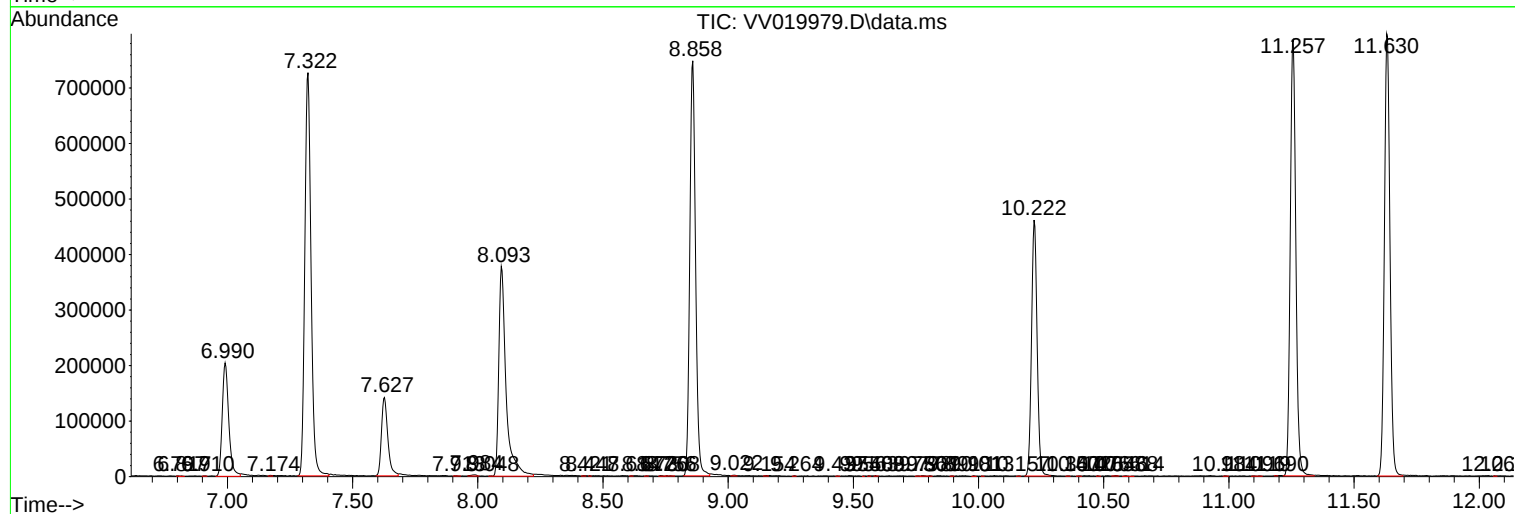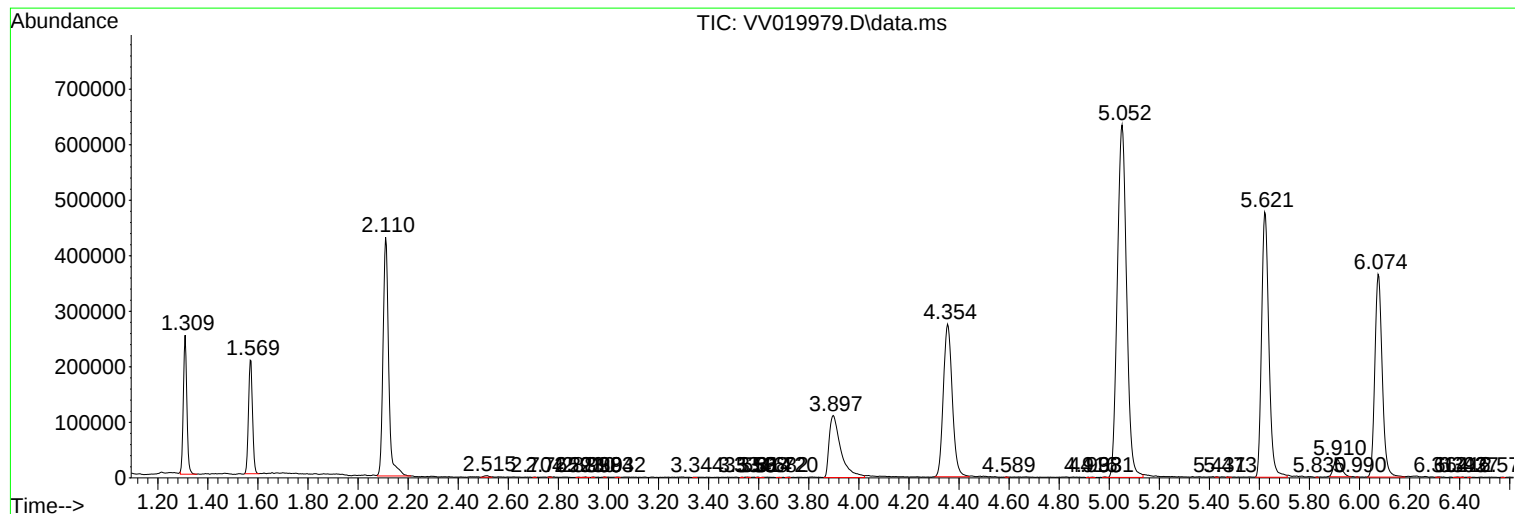

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011321\
Data File : VV019979.D
Acq On : 13 Jan 2021 11:03
Operator : SY/MD
Sample : VV0113WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK73

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011321\
Data File : VV019979.D
Acq On : 13 Jan 2021 11:03
Operator : SY/MD
Sample : VV0113WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK73

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
