
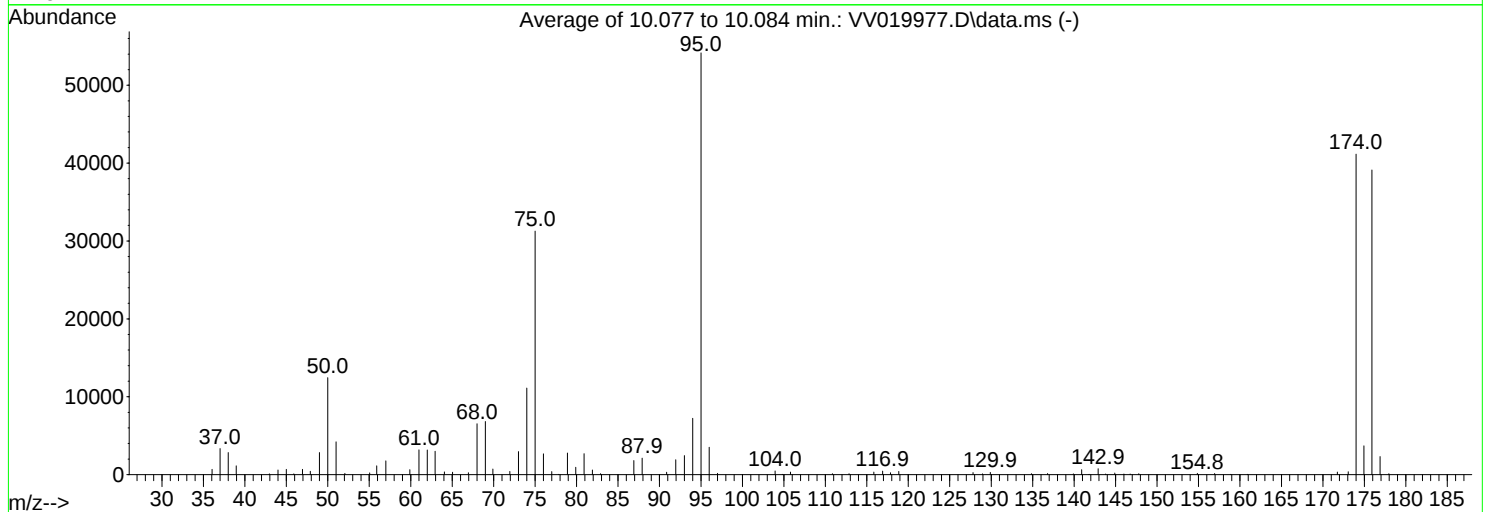


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011321\
 Data File : VV019977.D
 Acq On : 13 Jan 2021 09:20
 Operator : SY/MD
 Sample : BFB79
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB79

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
 Title : VOC Analysis
 Last Update : Sat Jan 16 04:43:48 2021

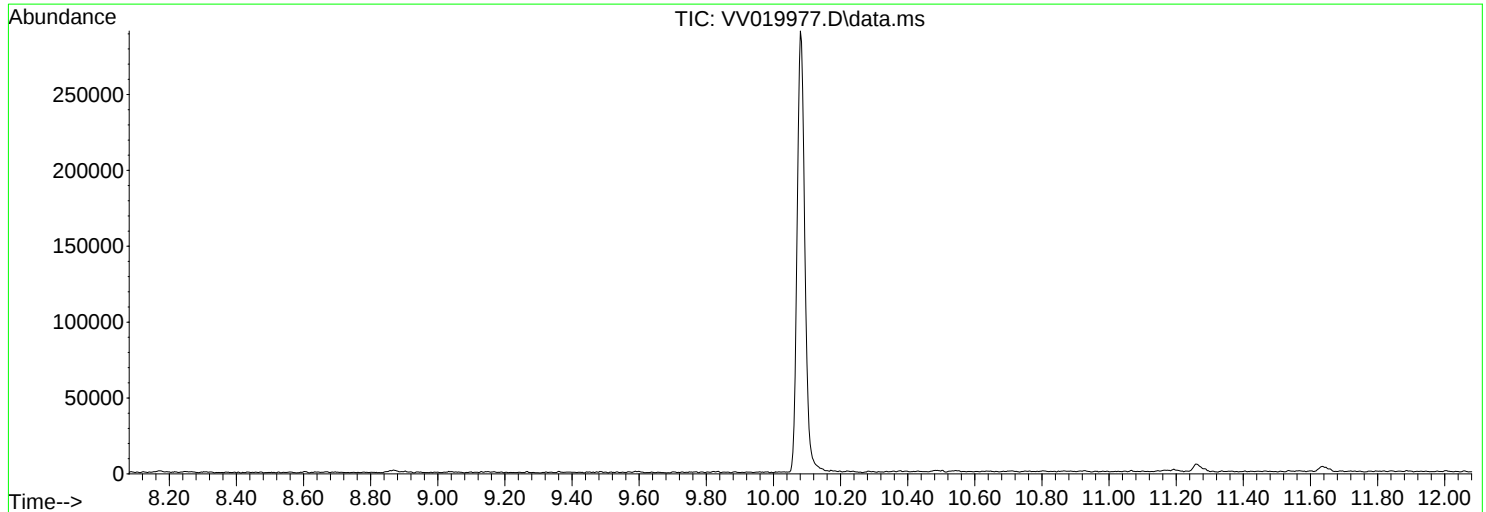

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	12454	PASS
75	95	30	80	57.7	31261	PASS
95	95	100	100	100.0	54160	PASS
96	95	5	9	6.5	3522	PASS
173	174	0.00	2	0.9	374	PASS
174	95	50	120	76.0	41163	PASS
175	174	5	9	9.0	3693	PASS
176	174	95	101	95.0	39123	PASS
177	176	5	9	6.0	2330	PASS

m/z	Abundance
38.00	102.0
38.90	175.0
40.00	311.0
44.00	457.0
78.00	103.0
96.70	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.10	584.0
37.00	3242.0
38.00	2994.0
39.00	1252.0
40.00	295.0
42.90	103.0
44.00	1062.0
45.00	643.0
45.90	158.0
46.90	699.0
47.90	432.0
49.00	2711.0
50.00	12316.0
51.00	4068.0
52.00	175.0
55.00	192.0
55.90	1127.0
57.00	1640.0
59.90	587.0
61.00	3192.0
62.00	3027.0
63.00	2934.0
64.10	354.0
65.10	272.0
66.90	257.0
68.00	6277.0
69.00	6379.0
69.90	685.0
71.90	436.0
73.00	2854.0
74.00	11241.0
75.00	30264.0
76.00	2486.0
77.00	351.0
77.80	110.0
78.90	2521.0
79.90	921.0
80.90	2594.0
81.90	499.0
82.90	112.0
86.90	1731.0
87.90	2044.0
90.90	261.0
92.00	1900.0
93.00	2322.0
94.00	6923.0
95.00	51696.0
96.00	3488.0
97.00	190.0
103.90	432.0
105.80	289.0
110.90	120.0
112.80	143.0
115.80	272.0
116.90	400.0
117.80	272.0
118.90	378.0
127.70	266.0
129.00	112.0
129.90	230.0
134.90	118.0
136.70	120.0
139.90	144.0
140.80	672.0
142.90	785.0
143.80	117.0
144.90	206.0
146.70	119.0
147.90	115.0
154.80	159.0
157.00	148.0
160.90	117.0
171.70	282.0
173.00	556.0
174.00	38344.0
175.00	3589.0
175.90	36712.0
176.90	2146.0
178.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	725.0
37.00	3478.0
38.00	2998.0
39.00	1344.0
40.00	299.0
43.00	108.0
44.00	1089.0
45.00	703.0
45.90	137.0
47.00	725.0
47.90	408.0
49.00	2979.0
50.00	12873.0
51.00	4290.0
52.10	160.0
55.00	244.0
55.90	1198.0
57.00	1770.0
59.90	658.0
61.00	3244.0
62.00	3260.0
62.90	3093.0
64.00	357.0
65.00	317.0
66.90	263.0
68.00	6811.0
69.00	7057.0
69.90	742.0
71.90	412.0
73.00	3076.0
74.00	11468.0
75.00	32280.0
76.00	2784.0
77.00	395.0
77.80	148.0
78.90	2862.0
79.90	981.0
80.90	2779.0
81.90	613.0
82.90	131.0
86.90	1849.0
87.90	2216.0
90.80	320.0
91.90	2020.0
93.00	2502.0
94.00	7447.0
95.00	56232.0
96.00	3557.0
97.00	163.0
104.00	521.0
105.80	332.0
110.80	117.0
112.80	118.0
115.80	339.0
116.90	479.0
117.80	245.0
118.90	434.0
127.80	278.0
128.90	112.0
129.90	330.0
134.90	106.0
136.80	148.0
139.90	140.0
140.90	623.0
142.90	791.0
143.80	113.0
144.90	230.0
146.00	115.0
146.80	133.0
147.90	125.0
154.80	149.0
156.90	136.0
171.70	330.0
173.10	566.0
174.00	42584.0
175.00	3862.0
175.90	40296.0
176.90	2420.0
178.00	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	755.0
37.00	3331.0
38.00	2825.0
39.00	1304.0
40.00	282.0
43.00	116.0
44.00	1040.0
45.00	677.0
47.00	634.0
47.90	439.0
49.00	2830.0
50.00	12173.0
51.00	4287.0
52.00	153.0
55.10	233.0
55.90	1089.0
57.00	1879.0
59.90	654.0
61.00	3136.0
62.00	3217.0
63.00	2949.0
64.00	361.0
65.00	347.0
67.00	198.0
68.00	6523.0
69.00	7033.0
69.90	711.0
72.00	357.0
73.00	2919.0
74.00	10664.0
75.00	31240.0
76.00	2744.0
77.00	427.0
77.80	211.0
78.90	2959.0
79.90	928.0
80.90	2721.0
81.90	674.0
82.90	102.0
86.90	1870.0
87.90	2100.0
90.80	370.0
91.90	1827.0
93.00	2505.0
94.00	7338.0
95.00	54552.0
96.00	3522.0
97.00	138.0
104.00	485.0
104.80	103.0
105.80	344.0
110.90	117.0
112.90	104.0
115.90	363.0
116.90	487.0
117.90	217.0
118.80	420.0
127.90	281.0
129.00	114.0
129.90	329.0
134.80	128.0
136.90	162.0
141.00	624.0
141.80	102.0
142.90	695.0
144.90	196.0
146.00	110.0
147.70	148.0
154.90	162.0
156.90	132.0
158.90	123.0
171.80	350.0
174.00	42560.0
174.90	3629.0
175.90	40360.0
176.90	2425.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79