


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024351.D
Acq On : 13 Jan 2022 15:49
Operator : SY/MD
Sample : N1084-03ME
Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLM6ME

Manual IntegrationsAPPROVED

Quant Time: Jan 13 22:25:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/20/2022
Supervised By :Mahesh Dadoda 01/20/2022

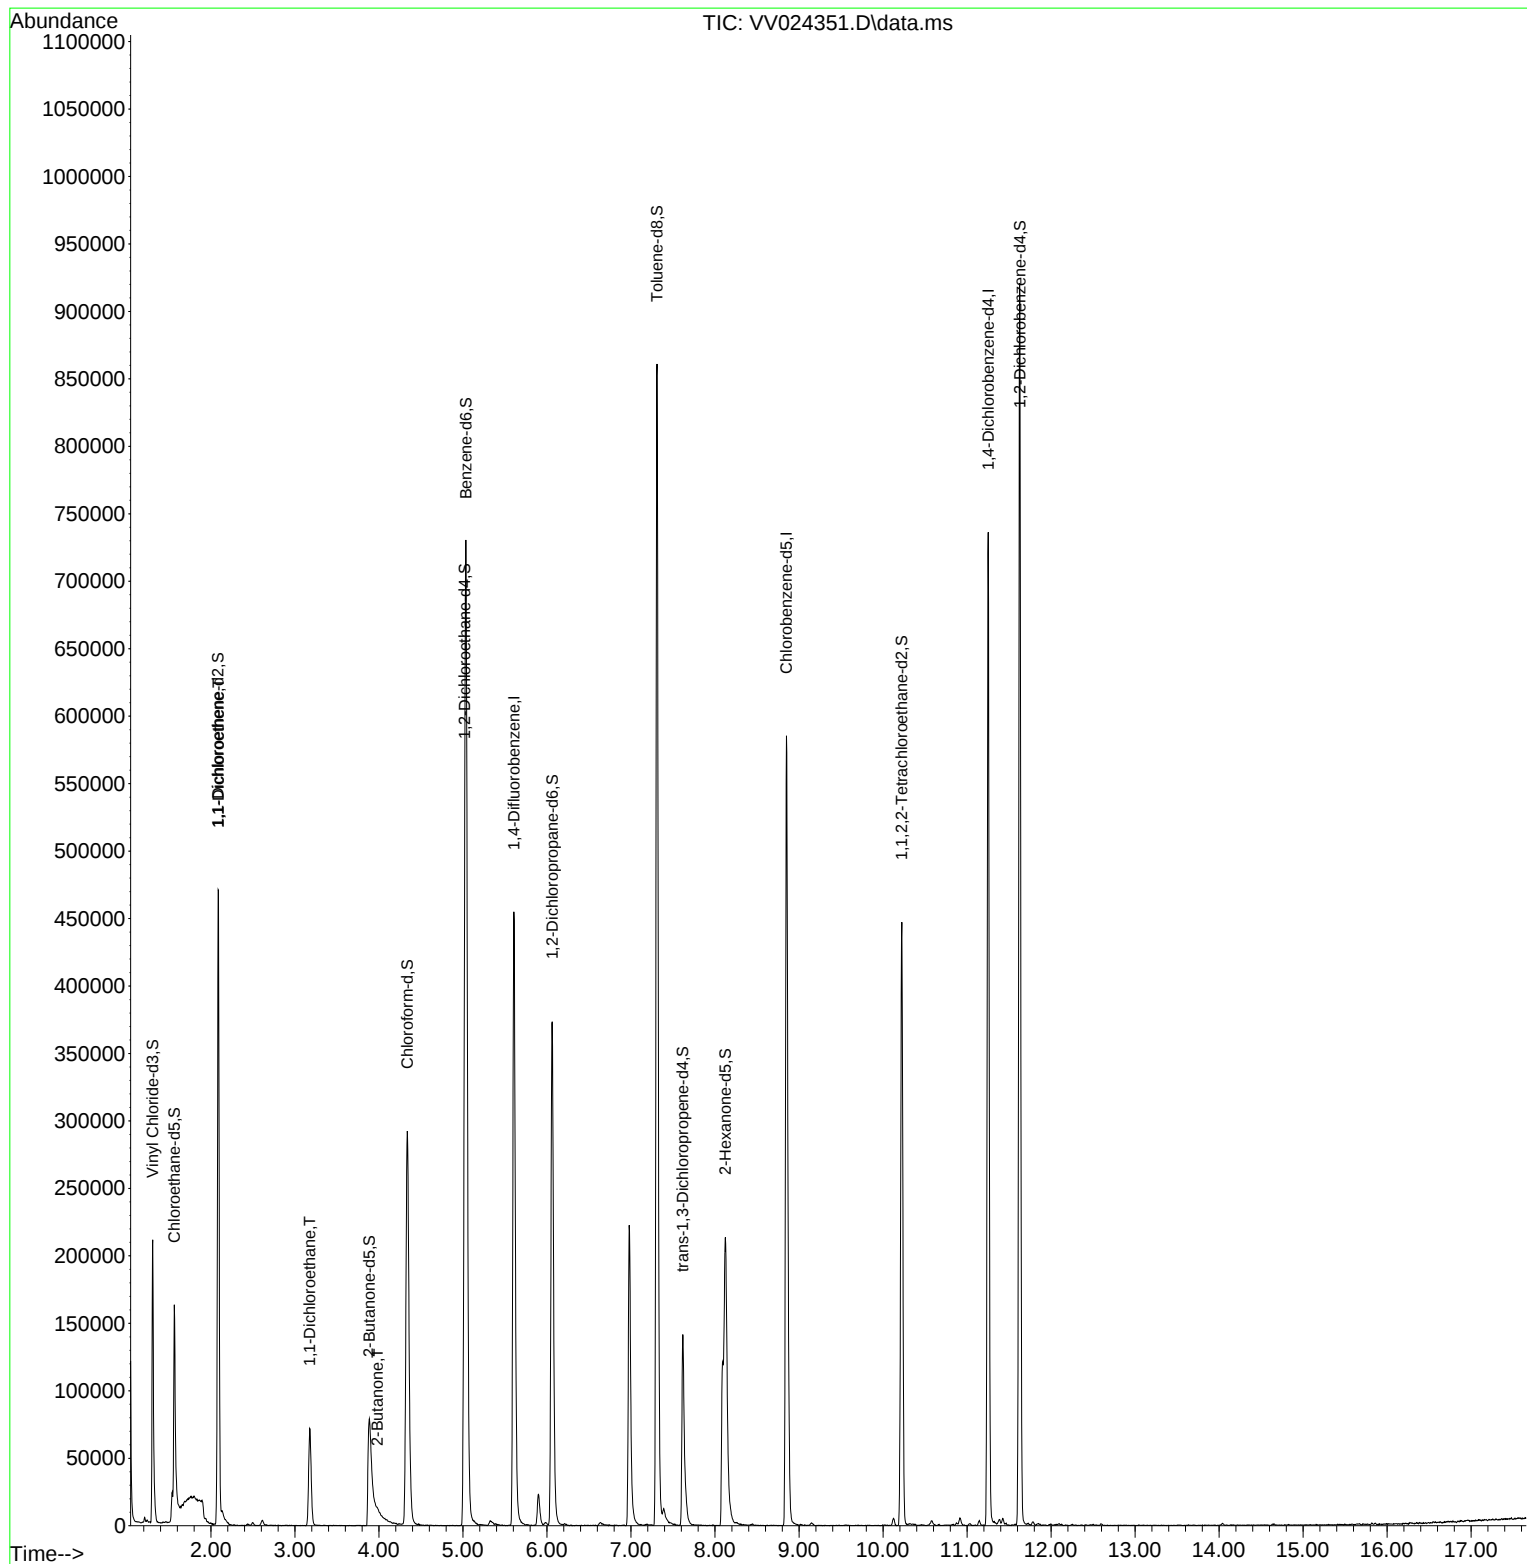




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024351.D
Acq On : 13 Jan 2022 15:49
Operator : SY/MD
Sample : N1084-03ME
Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLM6ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/20/2022
Supervised By :Mahesh Dadoda 01/20/2022

Quant Time: Jan 13 22:25:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

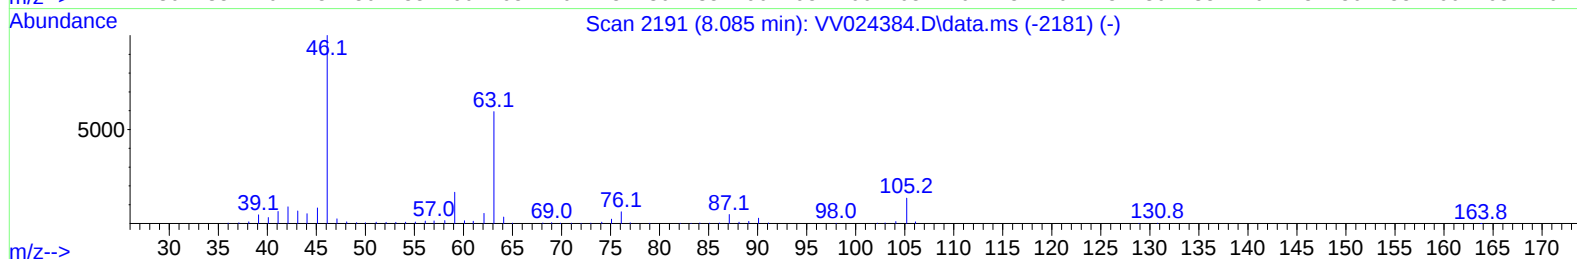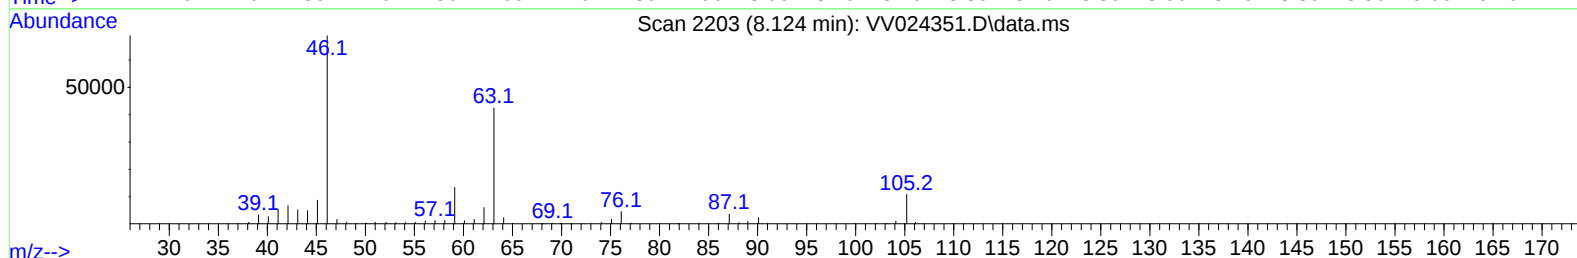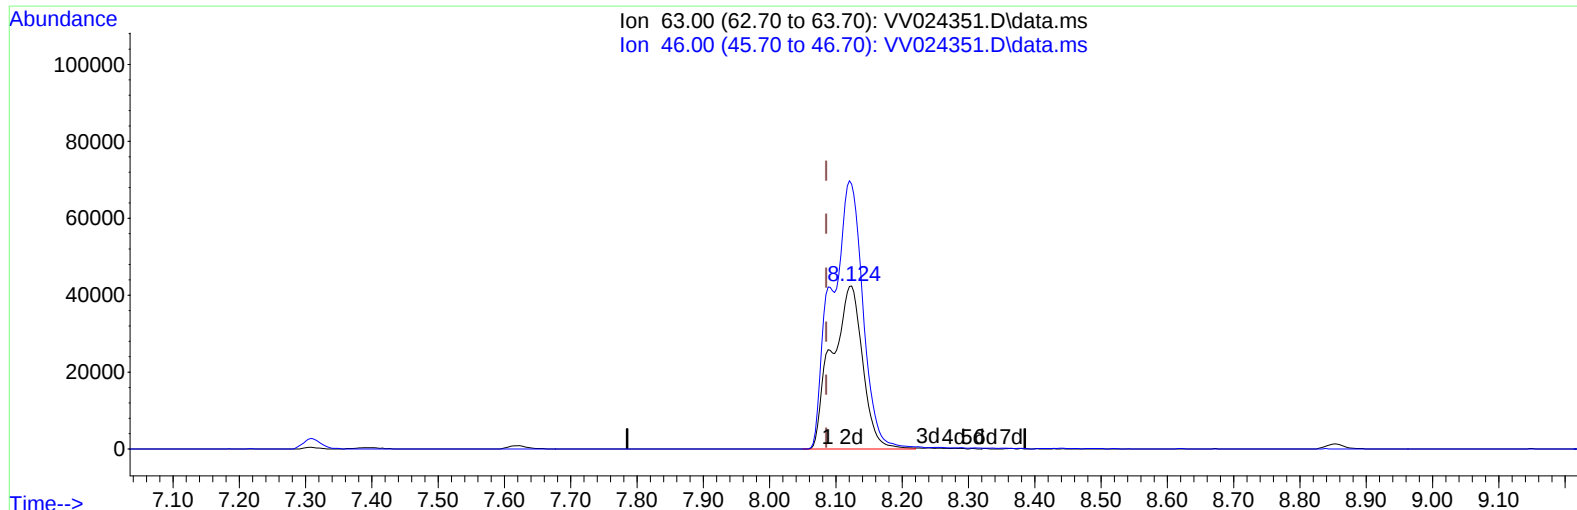

TIC: VV024351.D\data.ms

(47) 2-Hexanone-d5 (S)

8.124min (+ 0.038) 112.47 ug/L m

response 137271

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	169.00	42.63#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024351.D
Acq On : 13 Jan 2022 15:49
Operator : SY/MD
Sample : N1084-03ME
Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLM6ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/20/2022
Supervised By :Mahesh Dadoda 01/20/2022

Quant Time: Jan 21 22:33:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 21 00:04:44 2022
Response via : Initial Calibration

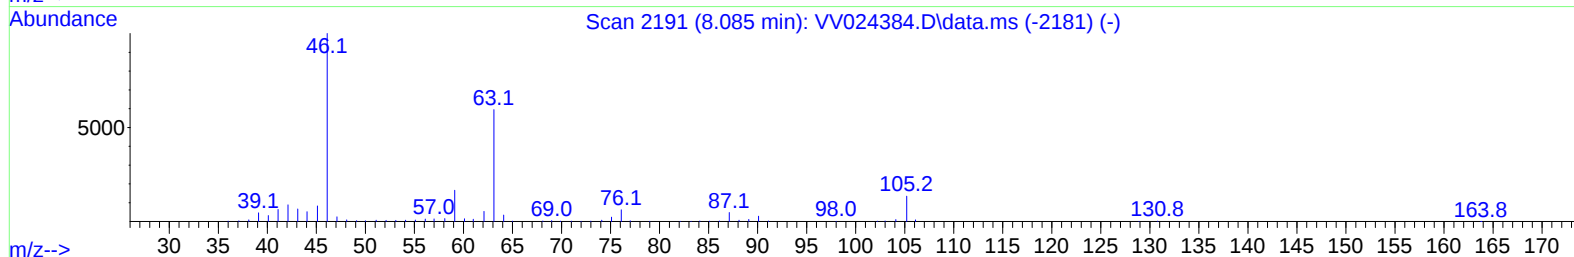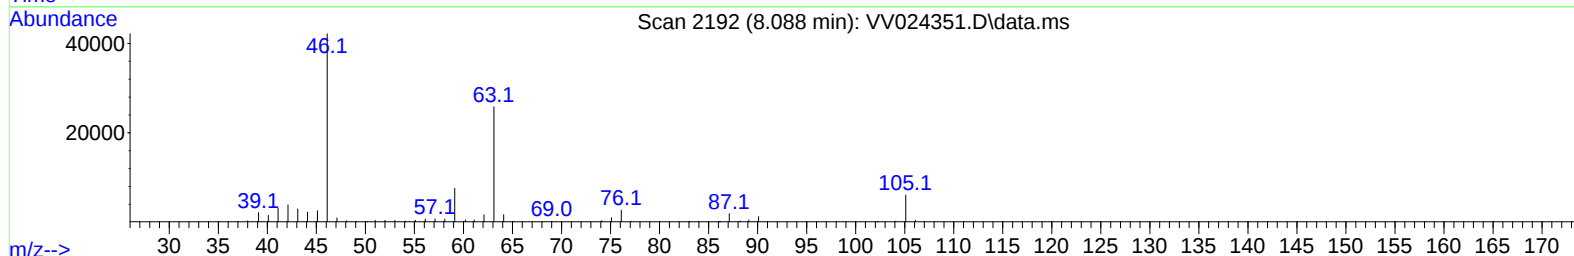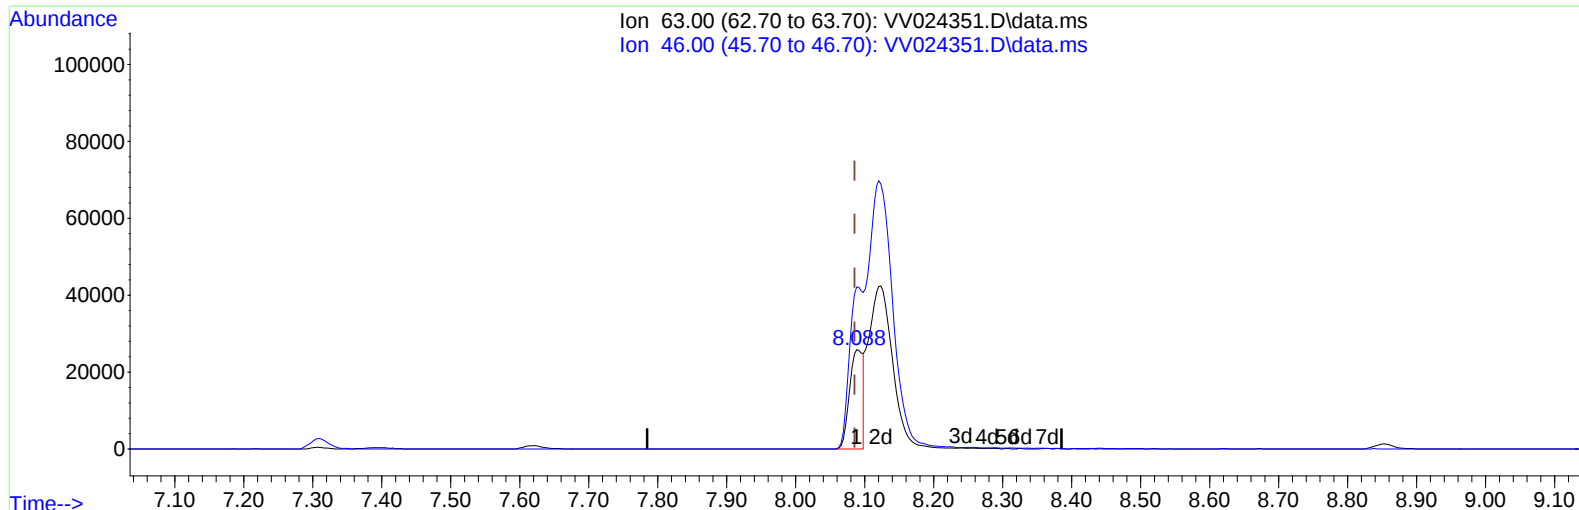

TIC: VV024351.D\data.ms

(47) 2-Hexanone-d5 (S)

8.088min (+ 0.003) 29.02 ug/L

response 35416

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	169.00	165.24
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024351.D
 Acq On : 13 Jan 2022 15:49
 Operator : SY/MD
 Sample : N1084-03ME
 Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLM6ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/20/2022
 Supervised By :Mahesh Dadoda 01/20/2022

Quant Time: Jan 13 22:25:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	409293	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	384121	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	200468	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	153978	52.273	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	= 104.540%		
7) Chloroethane-d5	1.564	69	112297	50.185	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	= 100.360%		
11) 1,1-Dichloroethene-d2	2.085	63	237979	43.227	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	= 86.460%		
21) 2-Butanone-d5	3.886	46	169960	103.562	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	= 103.560%		
24) Chloroform-d	4.336	84	297923	55.339	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 110.680%		
26) 1,2-Dichloroethane-d4	5.021	65	211294	58.620	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 117.240%		
32) Benzene-d6	5.037	84	609599	60.815	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 121.620%		
36) 1,2-Dichloropropane-d6	6.063	67	177809	63.294	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	= 126.580%#		
41) Toluene-d8	7.310	98	586236	60.403	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	= 120.800%#		
43) trans-1,3-Dichloroprop...	7.616	79	97402	60.212	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	= 120.420%		
47) 2-Hexanone-d5	8.124	63	137271m	112.471	ug/L	0.04
Spiked Amount 100.000	Range 45	- 130	Recovery	= 112.470%		
56) 1,1,2,2-Tetrachloroeth...	10.223	84	217871	54.269	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	= 108.540%		
66) 1,2-Dichlorobenzene-d4	11.628	152	246842	61.775	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	= 123.540%#		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.088	96	2622	1.052	ug/L #	1
19) 1,1-Dichloroethane	3.175	63	70488	16.542	ug/L	97
22) 2-Butanone	3.982	43	9515	5.528	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed