

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024349.D
 Acq On : 13 Jan 2022 14:06
 Operator : SY/MD
 Sample : VIBLK212
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK212

Quant Time: Jan 13 22:39:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	246587	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	232462	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	121487	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	80785	45.521	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.040%		
7) Chloroethane-d5	1.568	69	65091	48.282	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.560%		
11) 1,1-Dichloroethene-d2	2.108	63	121875	36.745	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.500%		
21) 2-Butanone-d5	3.880	46	99118	100.247	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	100.250%		
24) Chloroform-d	4.346	84	158229	48.784	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.560%		
26) 1,2-Dichloroethane-d4	5.027	65	105563	48.611	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.220%		
32) Benzene-d6	5.047	84	308519	50.858	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.720%		
36) 1,2-Dichloropropane-d6	6.066	67	90155	53.029	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	106.060%		
41) Toluene-d8	7.314	98	291769	49.676	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.360%		
43) trans-1,3-Dichloroprop...	7.619	79	45964	46.952	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.900%		
47) 2-Hexanone-d5	8.085	63	65989	89.341	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.340%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	113724	46.808	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.620%		
66) 1,2-Dichlorobenzene-d4	11.622	152	125352	51.765	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.540%		
Target Compounds					Qvalue	
48) 2-Hexanone	8.146	43	8993	6.176	ug/L #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024349.D
Acq On : 13 Jan 2022 14:06
Operator : SY/MD
Sample : VIBLK212
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK212

Quant Time: Jan 13 22:39:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

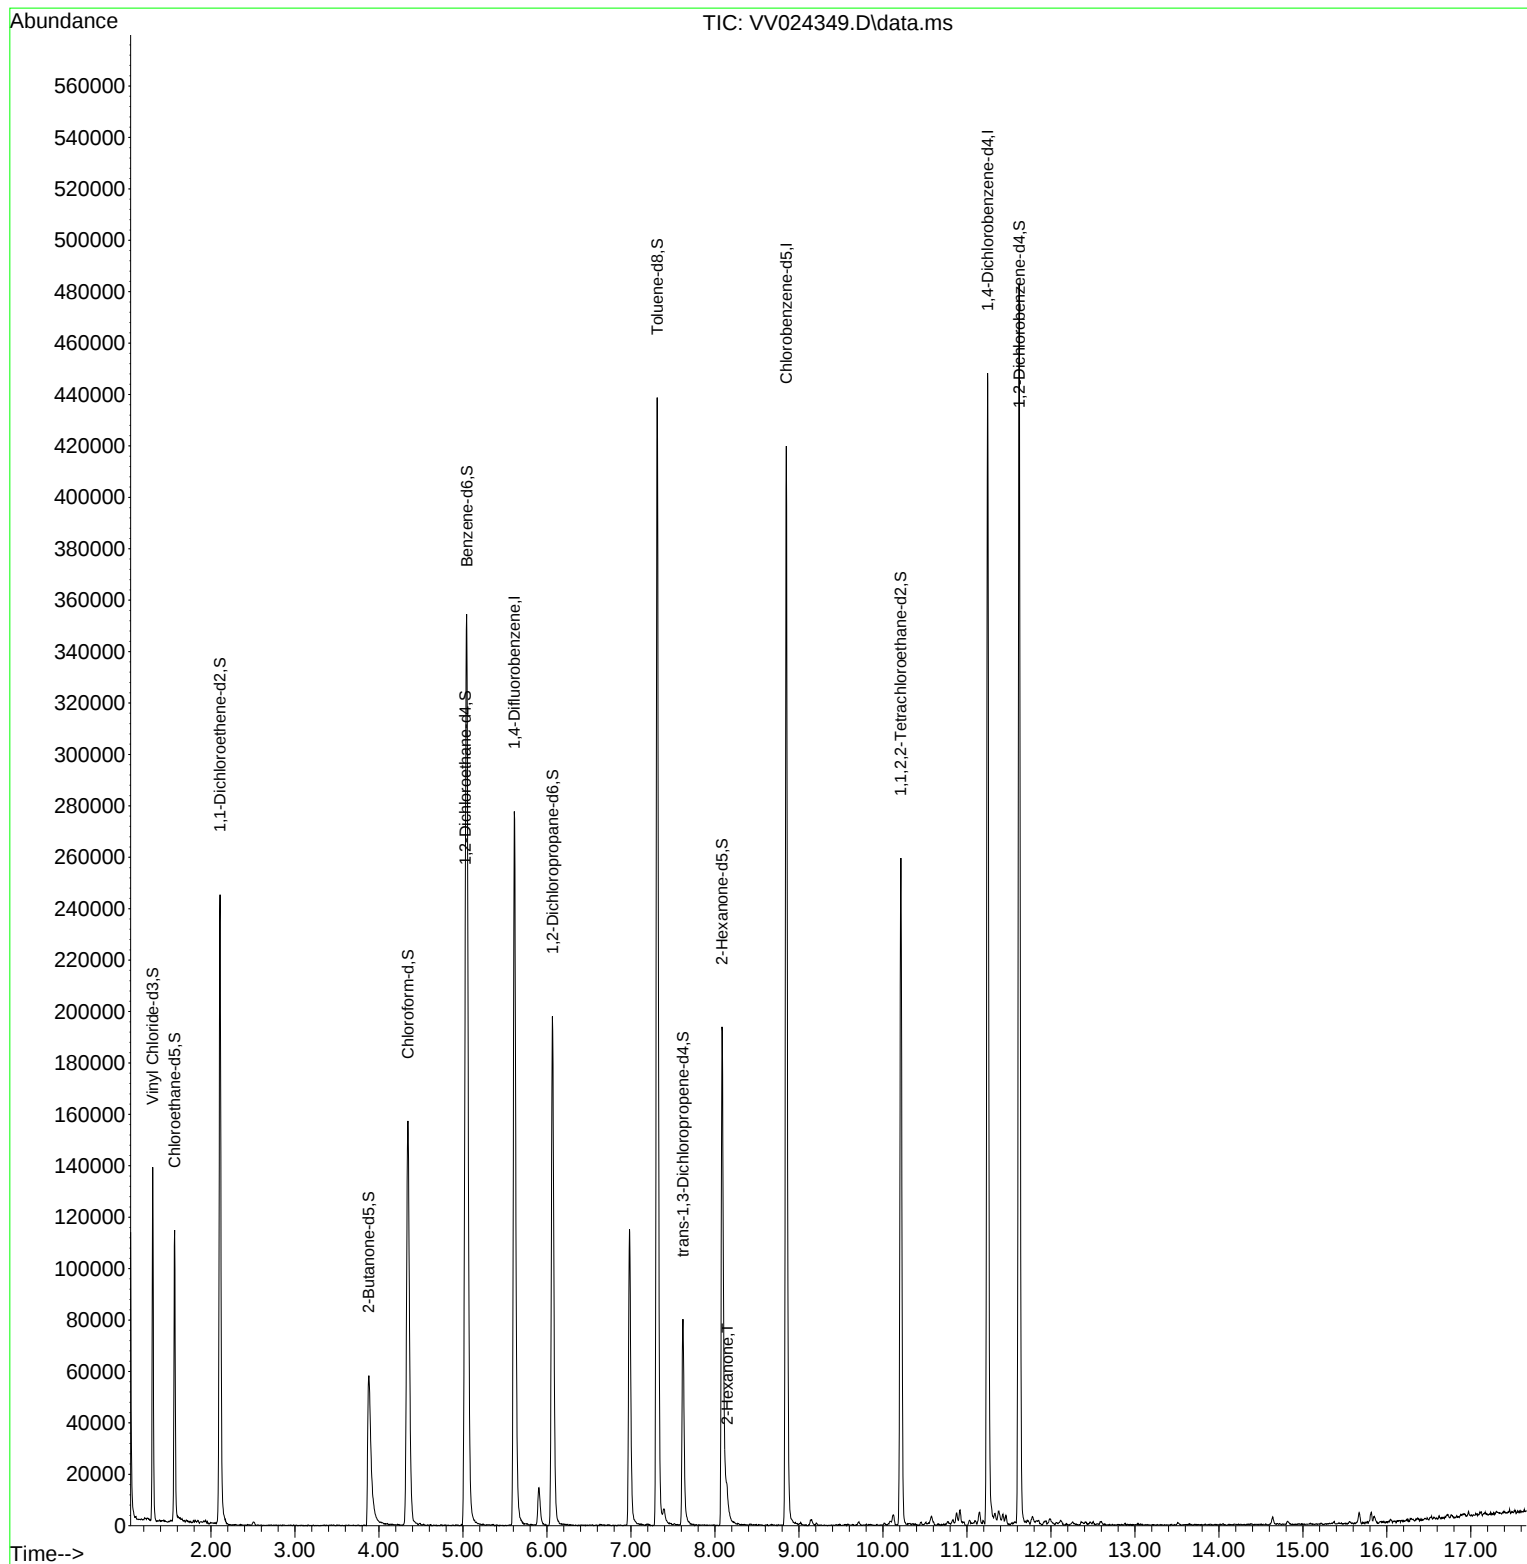

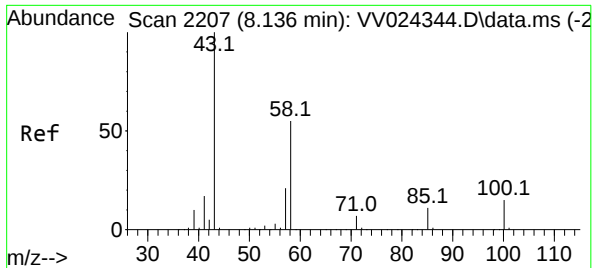

#48

2-Hexanone

Concen: 6.176 ug/L

RT: 8.146 min Scan# 21

Delta R.T. 0.010 min

Lab File: VV024349.D


Acq: 13 Jan 2022 14:06

Instrument :

MSVOA_V

ClientSampleId :

VIBLK212

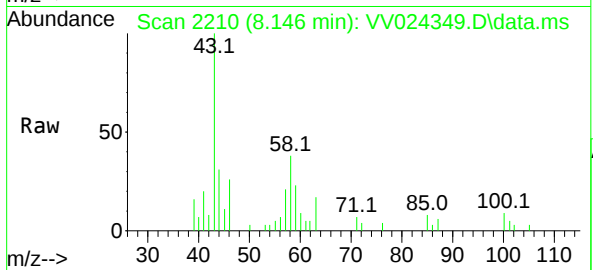

Tgt Ion: 43 Resp: 8993

Ion Ratio Lower Upper

43 100

58 42.0 45.0 67.4#

57 13.4 16.9 25.3#

100 2.9 13.0 19.4#

