

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024352.D
 Acq On : 13 Jan 2022 16:12
 Operator : SY/MD
 Sample : N1114-08ME
 Misc : 6.06g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLQ0ME

Quant Time: Jan 13 22:26:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	332424	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	312403	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	163351	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	113004	47.234	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.460%
7) Chloroethane-d5	1.564	69	87904	48.368	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.740%
11) 1,1-Dichloroethene-d2	2.101	63	180346	40.334	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.660%
21) 2-Butanone-d5	3.883	46	155307	116.517	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.520%
24) Chloroform-d	4.346	84	236780	54.152	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.300%
26) 1,2-Dichloroethane-d4	5.030	65	159605	54.519	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.040%
32) Benzene-d6	5.047	84	461994	56.670	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	113.340%
36) 1,2-Dichloropropane-d6	6.066	67	134417	58.833	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	117.660%
41) Toluene-d8	7.313	98	443530	56.191	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.380%
43) trans-1,3-Dichloroprop...	7.619	79	71581	54.409	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	108.820%
47) 2-Hexanone-d5	8.091	63	111052	111.877	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	111.880%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	175826	53.851	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	107.700%
66) 1,2-Dichlorobenzene-d4	11.625	152	192104	59.000	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	118.000%
Target Compounds						
					Qvalue	
46) Tetrachloroethene	7.976	164	9802	4.916	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024352.D
Acq On : 13 Jan 2022 16:12
Operator : SY/MD
Sample : N1114-08ME
Misc : 6.06g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLQ0ME

Quant Time: Jan 13 22:26:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

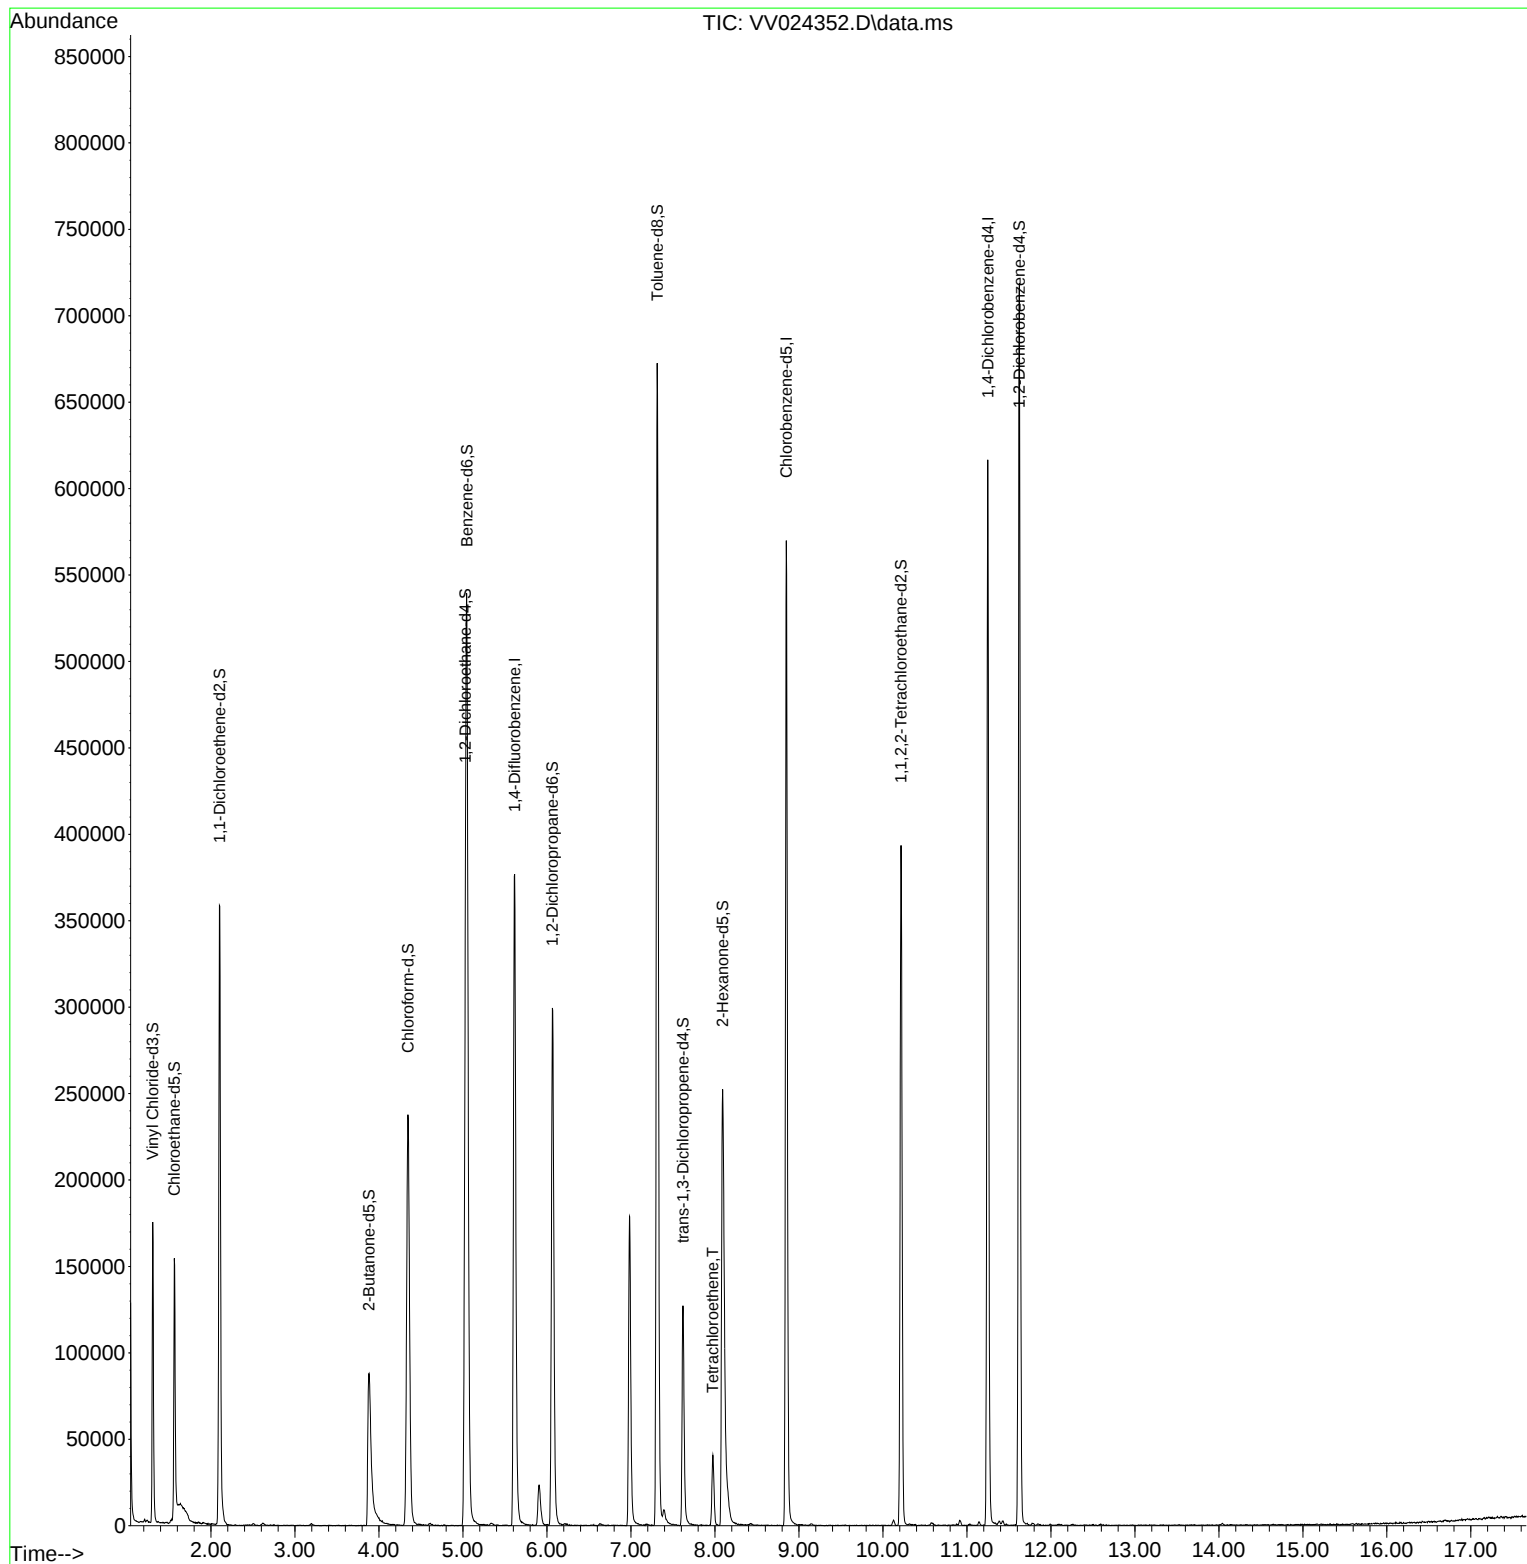

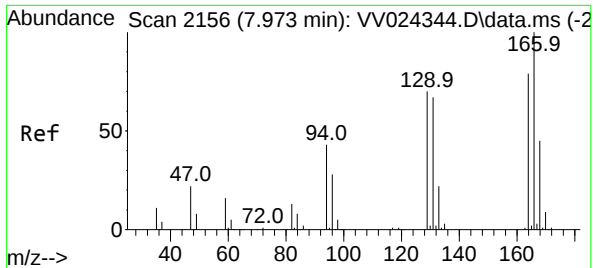

#46
 Tetrachloroethene
 Concen: 4.916 ug/L
 RT: 7.976 min Scan# 2156
 Delta R.T. 0.003 min
 Lab File: VV024352.D
 Acq: 13 Jan 2022 16:12

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLQ0ME

Tgt Ion:	164	Resp:	9802
Ion	Ratio	Lower	Upper
164	100		
129	90.2	61.5	114.1
131	87.0	62.2	115.4
166	140.0	89.9	166.9

