

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024354.D
 Acq On : 13 Jan 2022 17:09
 Operator : SY/MD
 Sample : N1132-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS9

Quant Time: Jan 13 22:26:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	238358	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	222014	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	111950	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	70734	41.234	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.460%
7) Chloroethane-d5	1.568	69	57137	43.846	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.700%
11) 1,1-Dichloroethene-d2	2.108	63	108343	33.793	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.580%
21) 2-Butanone-d5	3.876	46	83125	86.974	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.970%
24) Chloroform-d	4.342	84	143052	45.627	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.260%
26) 1,2-Dichloroethane-d4	5.027	65	95646	45.565	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.140%
32) Benzene-d6	5.047	84	281201	48.537	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.080%
36) 1,2-Dichloropropane-d6	6.066	67	81226	50.026	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.060%
41) Toluene-d8	7.313	98	261493	46.616	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.240%
43) trans-1,3-Dichloroprop...	7.619	79	43289	46.300	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.600%
47) 2-Hexanone-d5	8.085	63	59052	83.711	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.710%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	100386	43.263	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.520%
66) 1,2-Dichlorobenzene-d4	11.622	152	111360	49.905	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds						
13) Acetone	2.172	43	5448	5.773	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024354.D
Acq On : 13 Jan 2022 17:09
Operator : SY/MD
Sample : N1132-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS9

Quant Time: Jan 13 22:26:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

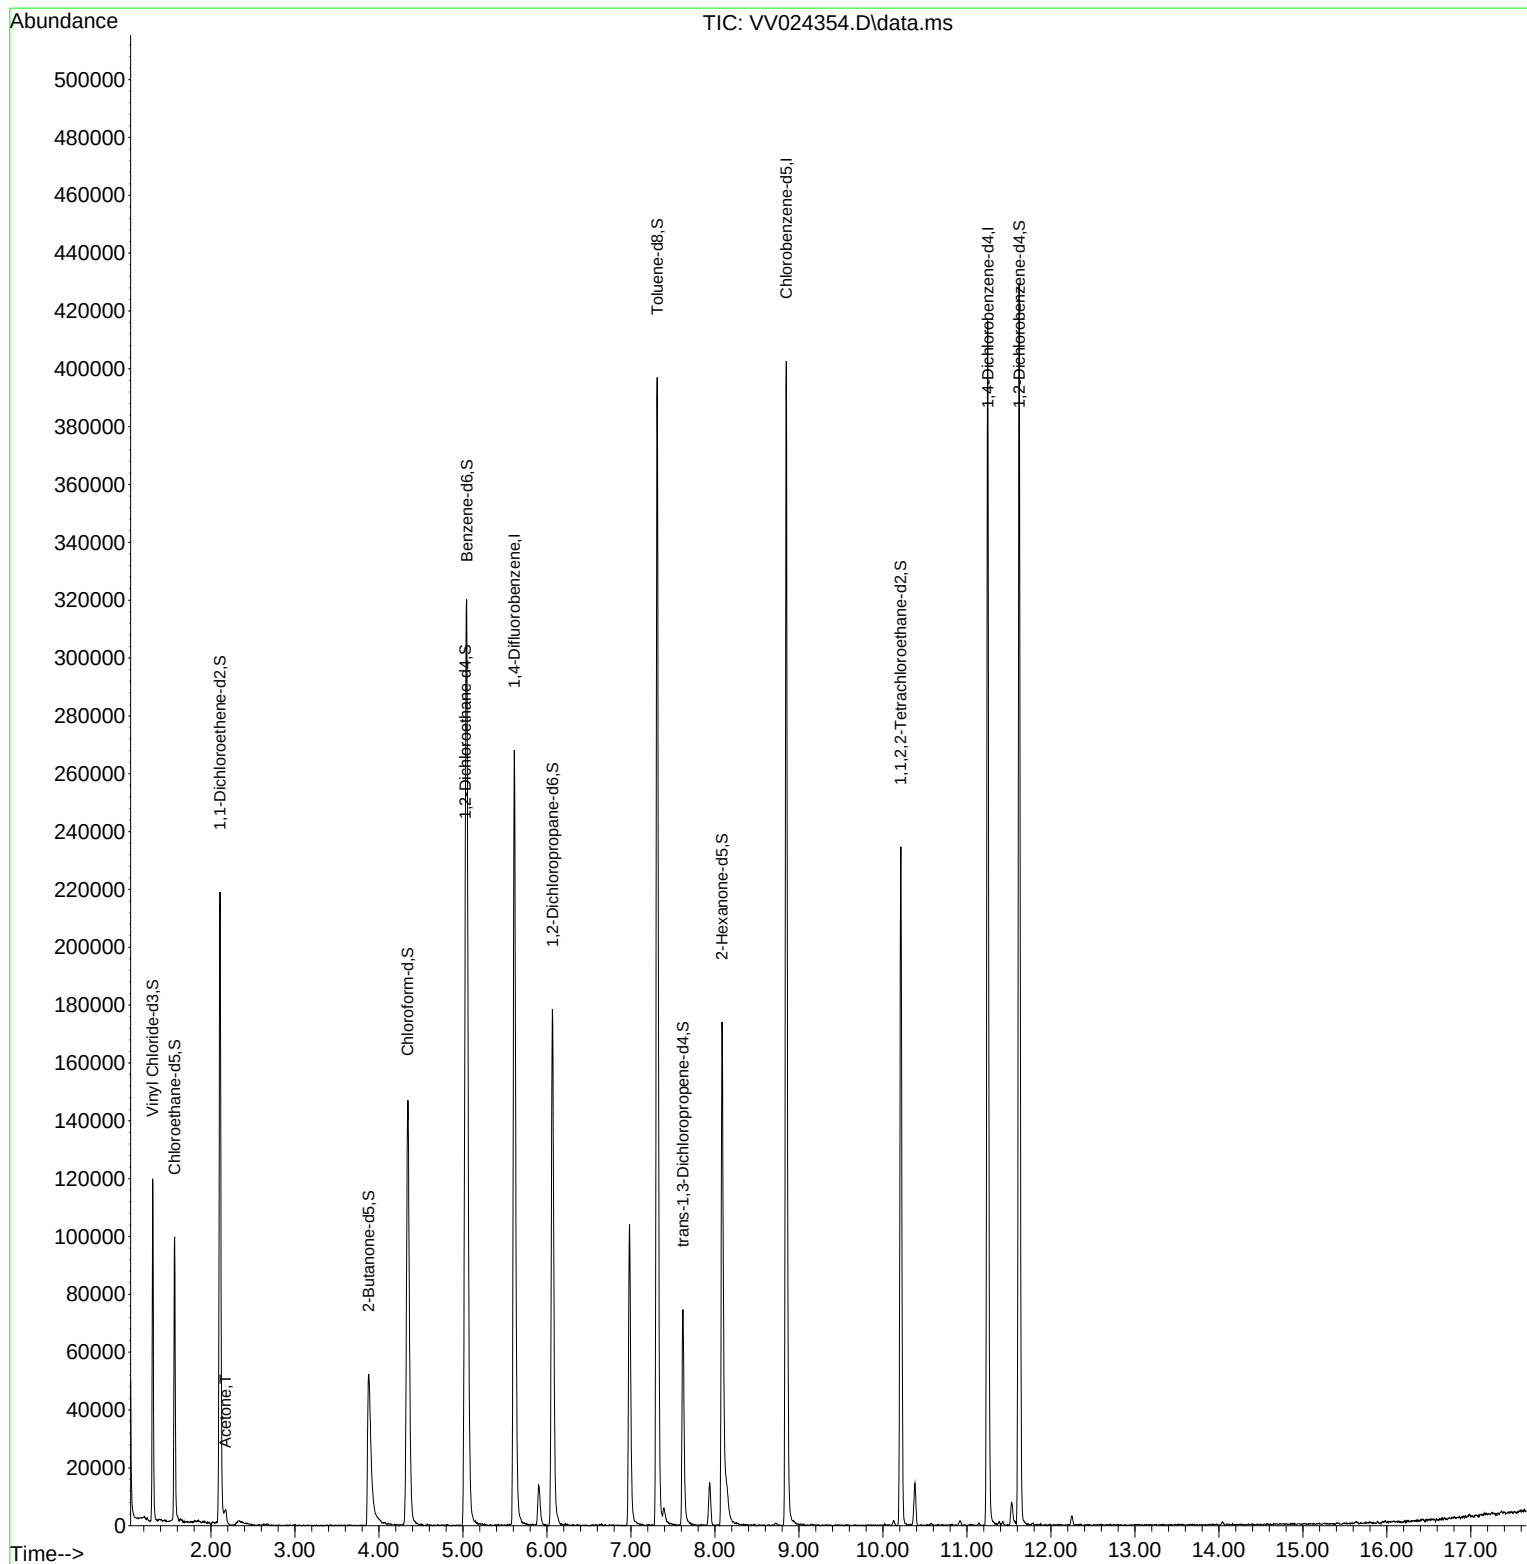

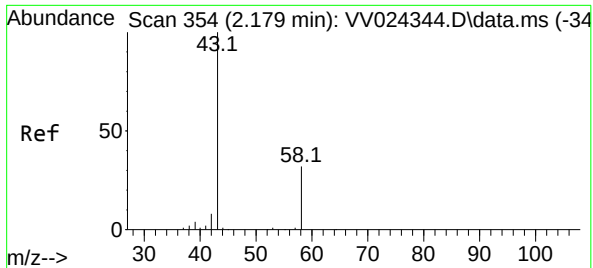

#13
 Acetone
 Concen: 5.773 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV024354.D
 Acq: 13 Jan 2022 17:09

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS9

Tgt Ion: 43 Resp: 5448
 Ion Ratio Lower Upper
 43 100
 58 35.5 0.0 63.0

