

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024356.D
 Acq On : 13 Jan 2022 17:57
 Operator : SY/MD
 Sample : N1115-16ME 10X
 Misc : 6.56g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS6ME

Quant Time: Jan 13 22:26:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	191459	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	179363	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	94320	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	91338	66.287	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	132.580%	
7) Chloroethane-d5	1.568	69	75446	72.077	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	144.160%#	
11) 1,1-Dichloroethene-d2	2.108	63	139702	54.248	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	108.500%	
21) 2-Butanone-d5	3.883	46	119473	155.626	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	155.630%#	
24) Chloroform-d	4.346	84	187963	74.638	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	149.280%#	
26) 1,2-Dichloroethane-d4	5.031	65	128455	76.185	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	152.380%#	
32) Benzene-d6	5.050	84	367964	78.615	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	157.220%#	
36) 1,2-Dichloropropane-d6	6.069	67	105821	80.671	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	161.340%#	
41) Toluene-d8	7.313	98	342523	75.581	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	151.160%#	
43) trans-1,3-Dichloroprop...	7.619	79	56053	74.208	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	148.420%#	
47) 2-Hexanone-d5	8.085	63	85565	150.139	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	150.140%#	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	140222	74.801	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	149.600%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	153418	81.604	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	163.200%#	
Target Compounds						
48) 2-Hexanone	8.146	43	10203	9.081	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024356.D
Acq On : 13 Jan 2022 17:57
Operator : SY/MD
Sample : N1115-16ME 10X
Misc : 6.56g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS6ME

Quant Time: Jan 13 22:26:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

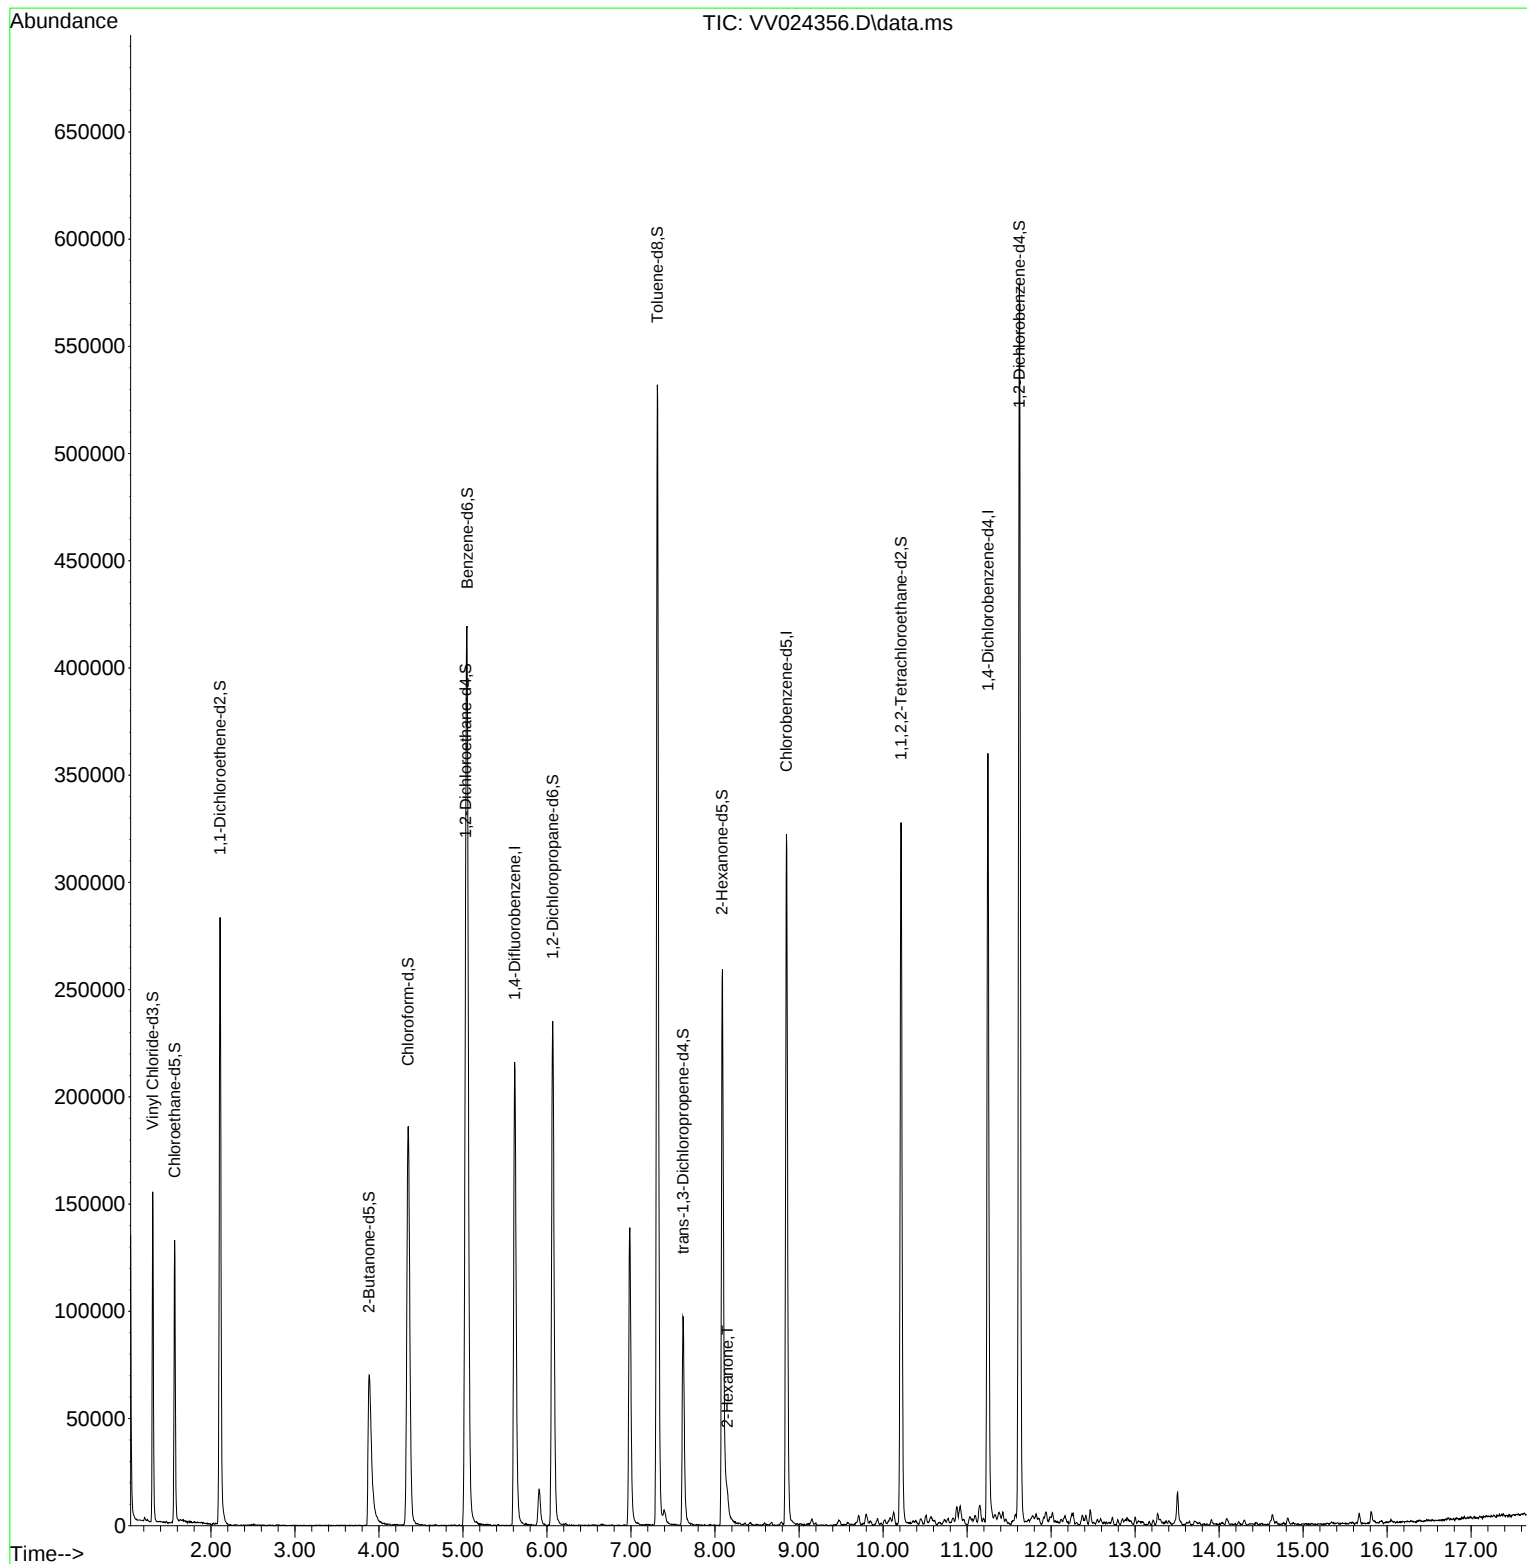

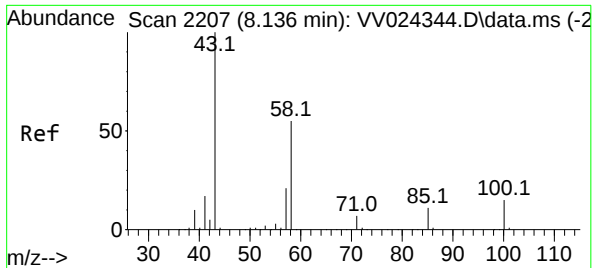

#48
 2-Hexanone
 Concen: 9.081 ug/L
 RT: 8.146 min Scan# 21
 Delta R.T. 0.010 min
 Lab File: VV024356.D
 Acq: 13 Jan 2022 17:57

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS6ME

Tgt Ion: 43	Resp:	10203
Ion	Ratio	Lower Upper
43	100	
58	30.8	45.0 67.4#
57	8.3	16.9 25.3#
100	7.3	13.0 19.4#

