

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
 Data File : VV024347.D
 Acq On : 13 Jan 2022 13:14
 Operator : SY/MD
 Sample : N1084-03ME
 Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLM6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M

Title : VOC Analysis

Signal : TIC: VV024347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	41040	49131	5.78%	0.897%
2	1.539	149	155	158	rBV	25710	29372	3.45%	0.536%
3	2.088	316	326	336	rBV	91288	131929	15.51%	2.408%
4	2.490	446	451	455	rBV5	1255	1616	0.19%	0.029%
5	2.603	481	486	487	rBV2	736	640	0.08%	0.012%
6	2.645	497	499	503	rVB	392	187	0.02%	0.003%
7	2.670	504	507	510	rBV2	281	247	0.03%	0.005%
8	2.789	540	544	546	rBV	258	188	0.02%	0.003%
9	2.815	550	552	555	rBV	241	163	0.02%	0.003%
10	2.889	572	575	578	rBV	164	155	0.02%	0.003%
11	3.175	649	664	687	rBV	131484	279495	32.86%	5.102%
12	3.313	705	707	713	rVV2	294	324	0.04%	0.006%
13	3.342	714	716	720	rVB2	275	202	0.02%	0.004%
14	3.603	793	797	801	rBV	157	194	0.02%	0.004%
15	3.683	819	822	824	rBV2	234	158	0.02%	0.003%
16	3.802	854	859	860	rBV	406	296	0.03%	0.005%
17	3.889	876	886	911	rBV	32838	111119	13.07%	2.028%
18	4.339	1011	1026	1051	rBV	83379	217400	25.56%	3.969%
19	4.445	1057	1059	1064	rVB3	582	295	0.03%	0.005%
20	4.526	1081	1084	1086	rVB	561	303	0.04%	0.006%
21	4.542	1086	1089	1092	rBB2	269	195	0.02%	0.004%
22	4.561	1093	1095	1098	rBV	298	201	0.02%	0.004%
23	4.628	1114	1116	1119	rVB	373	209	0.02%	0.004%
24	4.645	1119	1121	1125	rBV2	254	223	0.03%	0.004%
25	4.857	1184	1187	1190	rBB	286	198	0.02%	0.004%
26	4.889	1195	1197	1200	rBB	297	162	0.02%	0.003%
27	4.911	1201	1204	1207	rBV	311	321	0.04%	0.006%
28	5.034	1225	1242	1267	rBV2	181785	460845	54.19%	8.413%
29	5.461	1372	1375	1377	rVB	347	163	0.02%	0.003%
30	5.551	1394	1403	1407	rBV3	639	936	0.11%	0.017%
31	5.606	1407	1420	1456	rVV	347295	710776	83.58%	12.975%
32	5.844	1490	1494	1497	rBV2	369	328	0.04%	0.006%
33	5.902	1502	1512	1530	rBV5	9781	21255	2.50%	0.388%
34	5.985	1534	1538	1542	rBV4	1529	1517	0.18%	0.028%
35	6.063	1549	1562	1589	rVB	104426	223698	26.30%	4.084%
36	6.162	1589	1593	1596	rVB2	902	776	0.09%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024347.D
 Acq On : 13 Jan 2022 13:14
 Operator : SY/MD
 Sample : N1084-03ME
 Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLM6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	6.188	1596	1601	1606	rBV3	485	586	0.07%	0.011%
38	6.217	1606	1610	1613	rVB2	390	295	0.03%	0.005%
39	6.239	1614	1617	1622	rBV2	369	320	0.04%	0.006%
40	6.284	1629	1631	1634	rVB	351	156	0.02%	0.003%
41	6.387	1659	1663	1666	rBV	271	235	0.03%	0.004%
42	6.580	1719	1723	1726	rVB2	272	218	0.03%	0.004%
43	6.641	1734	1742	1747	rBV4	1561	2269	0.27%	0.041%
44	6.767	1778	1781	1783	rBV	390	210	0.02%	0.004%
45	6.853	1806	1808	1813	rVB2	538	374	0.04%	0.007%
46	6.882	1813	1817	1819	rBV	272	210	0.02%	0.004%
47	6.982	1838	1848	1869	rBV2	55632	112105	13.18%	2.046%
48	7.262	1933	1935	1938	rVB2	280	174	0.02%	0.003%
49	7.310	1938	1950	1969	rBV	172244	314347	36.96%	5.738%
50	7.519	2011	2015	2022	rBV3	660	684	0.08%	0.012%
51	7.571	2027	2031	2033	rVB2	253	185	0.02%	0.003%
52	7.622	2037	2047	2078	rBV	36153	79179	9.31%	1.445%
53	7.802	2100	2103	2107	rVB2	351	284	0.03%	0.005%
54	7.943	2142	2147	2154	rVB3	440	471	0.06%	0.009%
55	7.995	2161	2163	2168	rVB	383	276	0.03%	0.005%
56	8.046	2177	2179	2184	rVB	265	188	0.02%	0.003%
57	8.127	2184	2204	2233	rBV2	85511	289897	34.09%	5.292%
58	8.397	2284	2288	2291	rVB3	497	391	0.05%	0.007%
59	8.432	2295	2299	2302	rBV3	550	565	0.07%	0.010%
60	8.513	2321	2324	2327	rBV2	514	265	0.03%	0.005%
61	8.567	2339	2341	2344	rVB	301	155	0.02%	0.003%
62	8.603	2349	2352	2356	rBV2	203	183	0.02%	0.003%
63	8.715	2383	2387	2389	rVB	344	221	0.03%	0.004%
64	8.760	2399	2401	2405	rVB	274	175	0.02%	0.003%
65	8.850	2417	2429	2457	rBV	446139	850451	100.00%	15.525%
66	9.095	2500	2505	2508	rVB2	372	412	0.05%	0.008%
67	9.114	2508	2511	2514	rBV2	186	163	0.02%	0.003%
68	9.146	2516	2521	2528	rBV2	624	710	0.08%	0.013%
69	9.220	2541	2544	2551	rVB2	220	295	0.03%	0.005%
70	9.284	2561	2564	2567	rBV	165	172	0.02%	0.003%
71	9.403	2599	2601	2606	rVB	261	161	0.02%	0.003%
72	9.455	2612	2617	2620	rBV2	238	201	0.02%	0.004%
73	9.583	2654	2657	2663	rBV	220	283	0.03%	0.005%
74	9.783	2716	2719	2725	rVB	289	303	0.04%	0.006%
75	9.924	2759	2763	2765	rBV	263	215	0.03%	0.004%
76	9.956	2770	2773	2775	rBV	189	152	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024347.D
 Acq On : 13 Jan 2022 13:14
 Operator : SY/MD
 Sample : N1084-03ME
 Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLM6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	10.095	2813	2816	2819	rBV	216	176	0.02%	0.003%
78	10.162	2832	2837	2840	rBV2	304	367	0.04%	0.007%
79	10.223	2840	2856	2871	rBV	165111	297519	34.98%	5.431%
80	10.538	2952	2954	2956	rBV	345	184	0.02%	0.003%
81	10.583	2962	2968	2974	rVB4	1285	1631	0.19%	0.030%
82	10.622	2974	2980	2981	rBV2	246	216	0.03%	0.004%
83	10.744	3014	3018	3021	rBV2	312	269	0.03%	0.005%
84	10.799	3032	3035	3041	rBV2	240	200	0.02%	0.004%
85	10.914	3066	3071	3072	rBV2	432	271	0.03%	0.005%
86	11.252	3163	3176	3197	rBV	531254	837699	98.50%	15.292%
87	11.487	3247	3249	3254	rVB	517	252	0.03%	0.005%
88	11.564	3271	3273	3277	rBV2	229	183	0.02%	0.003%
89	11.628	3281	3293	3309	rBV	271830	433201	50.94%	7.908%
90	12.181	3462	3465	3471	rVB2	196	191	0.02%	0.003%
91	12.249	3484	3486	3493	rVB2	593	491	0.06%	0.009%
92	12.326	3506	3510	3513	rBV2	253	207	0.02%	0.004%
93	12.853	3669	3674	3677	rVB2	183	174	0.02%	0.003%
94	13.220	3785	3788	3794	rVB2	259	247	0.03%	0.005%
95	13.374	3832	3836	3837	rBV2	278	182	0.02%	0.003%
96	13.471	3863	3866	3870	rBV	208	193	0.02%	0.004%
97	13.506	3873	3877	3878	rBV2	533	374	0.04%	0.007%
98	13.995	4027	4029	4033	rBV2	265	176	0.02%	0.003%
99	14.155	4076	4079	4081	rBV	249	146	0.02%	0.003%
100	14.387	4150	4151	4158	rVB2	262	160	0.02%	0.003%




Sum of corrected areas: 5478062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024347.D
Acq On : 13 Jan 2022 13:14
Operator : SY/MD
Sample : N1084-03ME
Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLM6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

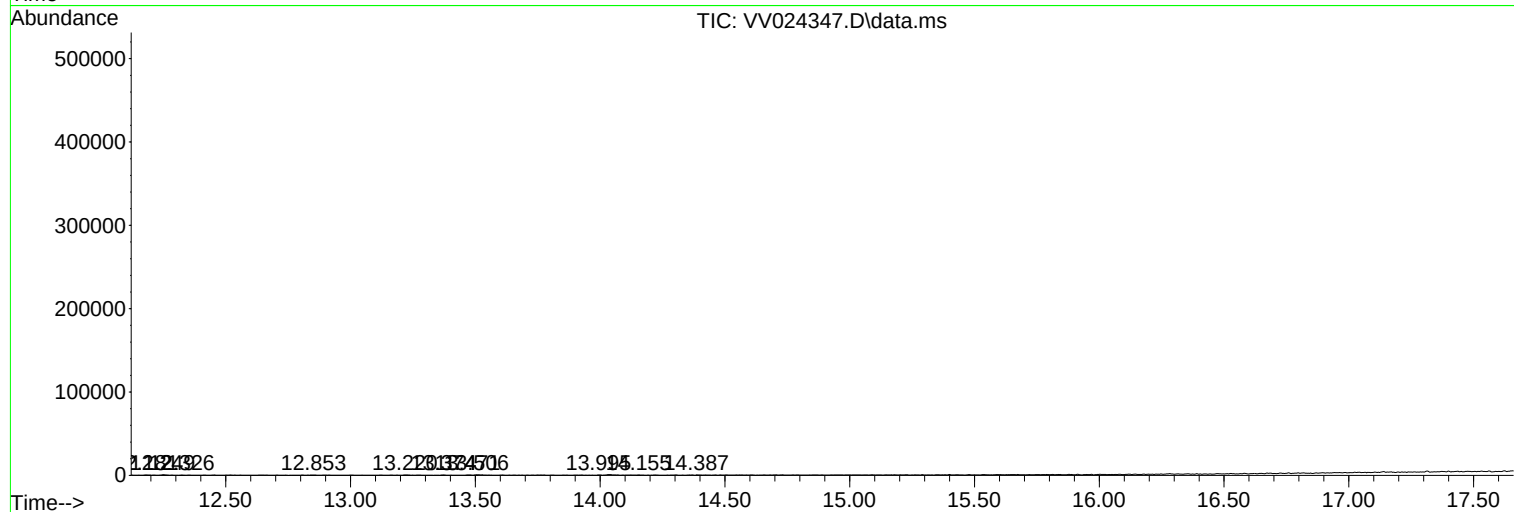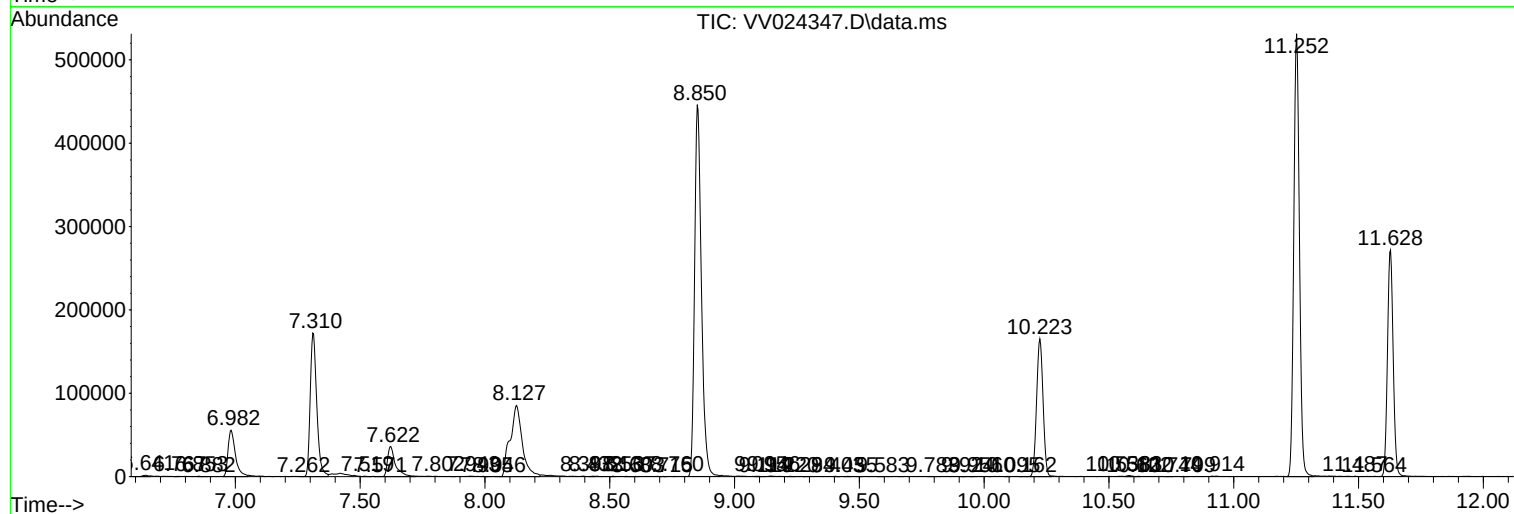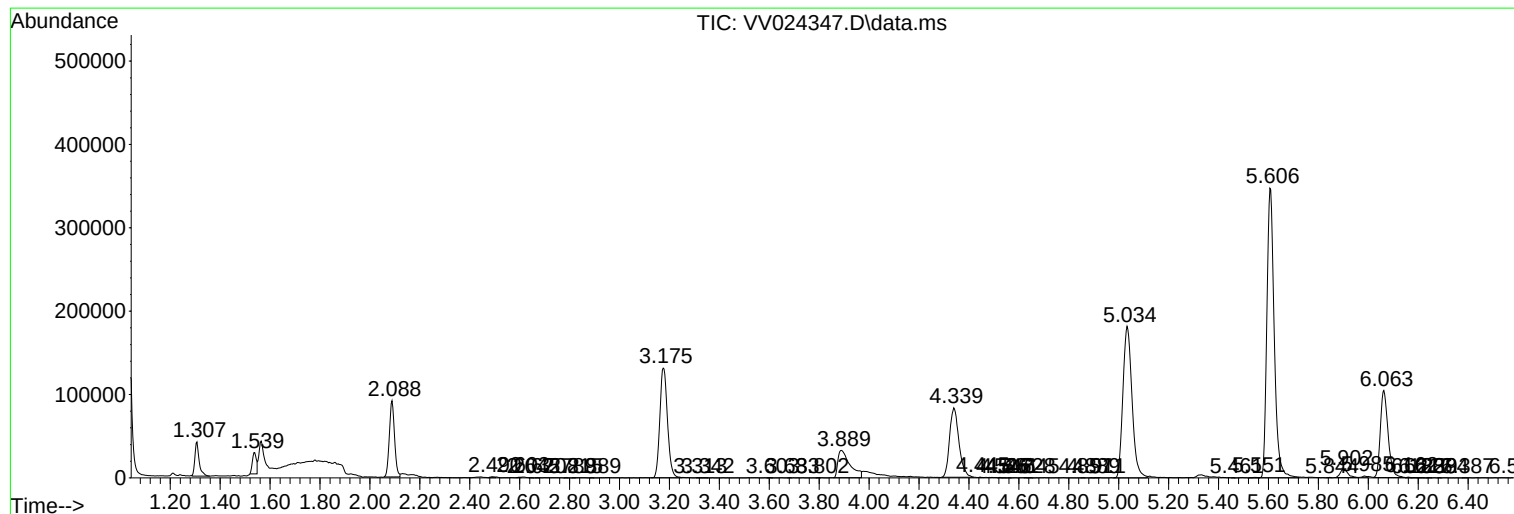

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024347.D
Acq On : 13 Jan 2022 13:14
Operator : SY/MD
Sample : N1084-03ME
Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLM6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024347.D
Acq On : 13 Jan 2022 13:14
Operator : SY/MD
Sample : N1084-03ME
Misc : 6.44g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLM6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------