

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024356.D
 Acq On : 13 Jan 2022 17:57
 Operator : SY/MD
 Sample : N1115-16ME 10X
 Misc : 6.56g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

Signal : TIC: VW024356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	153854	152836	13.95%	1.942%
2	1.568	157	164	178	rVB	130842	143250	13.07%	1.821%
3	2.108	321	332	358	rBV	282842	409550	37.37%	5.205%
4	2.359	406	410	414	rVB2	362	382	0.03%	0.005%
5	2.507	455	456	459	rBV	477	267	0.02%	0.003%
6	2.667	503	506	509	rBV	248	211	0.02%	0.003%
7	2.703	514	517	518	rVV	384	242	0.02%	0.003%
8	2.732	521	526	530	rVB2	307	402	0.04%	0.005%
9	2.780	537	541	543	rBV2	432	341	0.03%	0.004%
10	2.976	597	602	605	rBV2	269	356	0.03%	0.005%
11	3.066	626	630	632	rBV	234	207	0.02%	0.003%
12	3.362	720	722	727	rVB2	264	240	0.02%	0.003%
13	3.404	731	735	738	rVB	370	302	0.03%	0.004%
14	3.674	815	819	823	rBB2	280	249	0.02%	0.003%
15	3.716	829	832	840	rBB2	340	375	0.03%	0.005%
16	3.764	841	847	849	rBV2	308	346	0.03%	0.004%
17	3.838	861	870	872	rBV	311	367	0.03%	0.005%
18	3.883	872	884	924	rBV2	70141	212429	19.38%	2.700%
19	4.349	1013	1029	1058	rBV	185630	459706	41.95%	5.842%
20	4.606	1107	1109	1112	rBB2	366	247	0.02%	0.003%
21	4.645	1119	1121	1125	rBV2	268	262	0.02%	0.003%
22	4.667	1126	1128	1131	rVV	499	308	0.03%	0.004%
23	4.687	1131	1134	1138	rVV2	312	265	0.02%	0.003%
24	4.744	1147	1152	1155	rBV2	269	295	0.03%	0.004%
25	4.834	1176	1180	1184	rBV2	277	293	0.03%	0.004%
26	4.905	1200	1202	1205	rVB	448	252	0.02%	0.003%
27	4.960	1217	1219	1226	rVB	397	262	0.02%	0.003%
28	5.047	1227	1246	1277	rBV2	419545	1095893	100.00%	13.928%
29	5.407	1353	1358	1359	rBV	267	209	0.02%	0.003%
30	5.416	1359	1361	1366	rVB2	462	371	0.03%	0.005%
31	5.510	1385	1390	1395	rBB2	289	340	0.03%	0.004%
32	5.564	1403	1407	1410	rBV2	347	295	0.03%	0.004%
33	5.616	1411	1423	1449	rBV	216043	431644	39.39%	5.486%
34	5.905	1502	1513	1530	rBV3	16722	34865	3.18%	0.443%
35	6.069	1549	1564	1599	rBV	235294	483673	44.14%	6.147%
36	6.294	1629	1634	1639	rVV3	319	235	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011322\
 Data File : VW024356.D
 Acq On : 13 Jan 2022 17:57
 Operator : SY/MD
 Sample : N1115-16ME 10X
 Misc : 6.56g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	6.330	1642	1645	1649	rBV2	277	269	0.02%	0.003%
38	6.352	1650	1652	1658	rVB	285	209	0.02%	0.003%
39	6.645	1739	1743	1744	rBV2	511	374	0.03%	0.005%
40	6.918	1826	1828	1830	rVB	386	205	0.02%	0.003%
41	6.985	1836	1849	1872	rBV	139037	252948	23.08%	3.215%
42	7.188	1908	1912	1914	rBV4	413	342	0.03%	0.004%
43	7.313	1940	1951	1971	rBV	531299	898223	81.96%	11.415%
44	7.567	2026	2030	2035	rBV2	375	324	0.03%	0.004%
45	7.619	2035	2046	2070	rBV	97293	171047	15.61%	2.174%
46	7.937	2142	2145	2148	rBV2	471	349	0.03%	0.004%
47	8.088	2179	2192	2222	rBV	259500	490946	44.80%	6.239%
48	8.410	2285	2292	2294	rBV3	1197	1197	0.11%	0.015%
49	8.490	2312	2317	2320	rBV4	575	627	0.06%	0.008%
50	8.751	2395	2398	2402	rBV2	337	209	0.02%	0.003%
51	8.789	2402	2410	2418	rBV5	1537	2606	0.24%	0.033%
52	8.850	2418	2429	2447	rBV	322116	518560	47.32%	6.590%
53	9.005	2474	2477	2478	rBV	373	212	0.02%	0.003%
54	9.059	2491	2494	2496	rBV	629	297	0.03%	0.004%
55	9.095	2501	2505	2506	rBV	698	393	0.04%	0.005%
56	9.153	2514	2523	2531	rBV7	2817	4548	0.42%	0.058%
57	9.313	2569	2573	2576	rBV	359	314	0.03%	0.004%
58	9.374	2586	2592	2596	rBV2	331	486	0.04%	0.006%
59	9.407	2600	2602	2603	rBV	422	224	0.02%	0.003%
60	9.474	2614	2623	2632	rVV9	2426	4750	0.43%	0.060%
61	9.545	2640	2645	2647	rBV4	488	486	0.04%	0.006%
62	9.574	2652	2654	2655	rBV	729	307	0.03%	0.004%
63	9.661	2678	2681	2683	rBV	760	477	0.04%	0.006%
64	9.677	2683	2686	2688	rBV3	1017	764	0.07%	0.010%
65	9.747	2705	2708	2709	rBV2	527	220	0.02%	0.003%
66	9.799	2717	2724	2732	rBV6	4609	7827	0.71%	0.099%
67	9.905	2754	2757	2758	rBV	427	225	0.02%	0.003%
68	9.979	2774	2780	2784	rBV3	773	740	0.07%	0.009%
69	10.021	2786	2793	2798	rBV5	2159	3099	0.28%	0.039%
70	10.165	2836	2838	2841	rBV3	754	438	0.04%	0.006%
71	10.214	2842	2853	2875	rVV	327277	518051	47.27%	6.584%
72	10.452	2919	2927	2934	rBV10	2536	4350	0.40%	0.055%
73	10.513	2939	2946	2954	rBV5	3855	5470	0.50%	0.070%
74	10.664	2987	2993	2995	rBV5	1075	1265	0.12%	0.016%
75	11.034	3099	3108	3113	rBV8	3901	6634	0.61%	0.084%
76	11.249	3165	3175	3195	rBV	358122	543423	49.59%	6.906%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
 Data File : VV024356.D
 Acq On : 13 Jan 2022 17:57
 Operator : SY/MD
 Sample : N1115-16ME 10X
 Misc : 6.56g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	11.532	3260	3263	3265	rBV3	1491	1038	0.09%	0.013%
78	11.622	3281	3291	3311	rVB	577606	922891	84.21%	11.729%
79	12.374	3516	3525	3529	rBV8	4375	6735	0.61%	0.086%
80	12.464	3546	3553	3563	rBV4	6838	9833	0.90%	0.125%
81	12.551	3573	3580	3584	rBV7	2344	3086	0.28%	0.039%
82	12.792	3650	3655	3664	rBV8	2614	3558	0.32%	0.045%
83	12.850	3664	3673	3677	rBV6	3001	4539	0.41%	0.058%
84	13.001	3714	3720	3726	rBV4	3317	4027	0.37%	0.051%
85	13.169	3767	3772	3780	rVB5	1812	2193	0.20%	0.028%
86	13.217	3780	3787	3795	rBV4	2431	3383	0.31%	0.043%
87	13.268	3795	3803	3809	rBV6	5248	8147	0.74%	0.104%
88	13.680	3929	3931	3933	rBV2	468	278	0.03%	0.004%
89	13.705	3935	3939	3940	rBV3	1501	985	0.09%	0.013%
90	13.908	3994	4002	4006	rBV4	2553	3166	0.29%	0.040%
91	14.095	4052	4060	4068	rBV9	3008	5607	0.51%	0.071%
92	14.143	4073	4075	4076	rBV	506	236	0.02%	0.003%
93	14.258	4109	4111	4114	rBV	529	301	0.03%	0.004%
94	14.297	4118	4123	4124	rBV3	1654	1366	0.12%	0.017%
95	14.439	4164	4167	4172	rBV4	919	913	0.08%	0.012%
96	14.619	4216	4223	4224	rBV5	1997	2116	0.19%	0.027%
97	14.763	4266	4268	4270	rBV2	620	309	0.03%	0.004%
98	15.448	4479	4481	4485	rBV3	552	355	0.03%	0.005%
99	15.709	4560	4562	4564	rBV2	658	277	0.03%	0.004%
100	15.808	4588	4593	4603	rBV3	5312	7956	0.73%	0.101%


Sum of corrected areas: 7868497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024356.D
Acq On : 13 Jan 2022 17:57
Operator : SY/MD
Sample : N1115-16ME 10X
Misc : 6.56g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

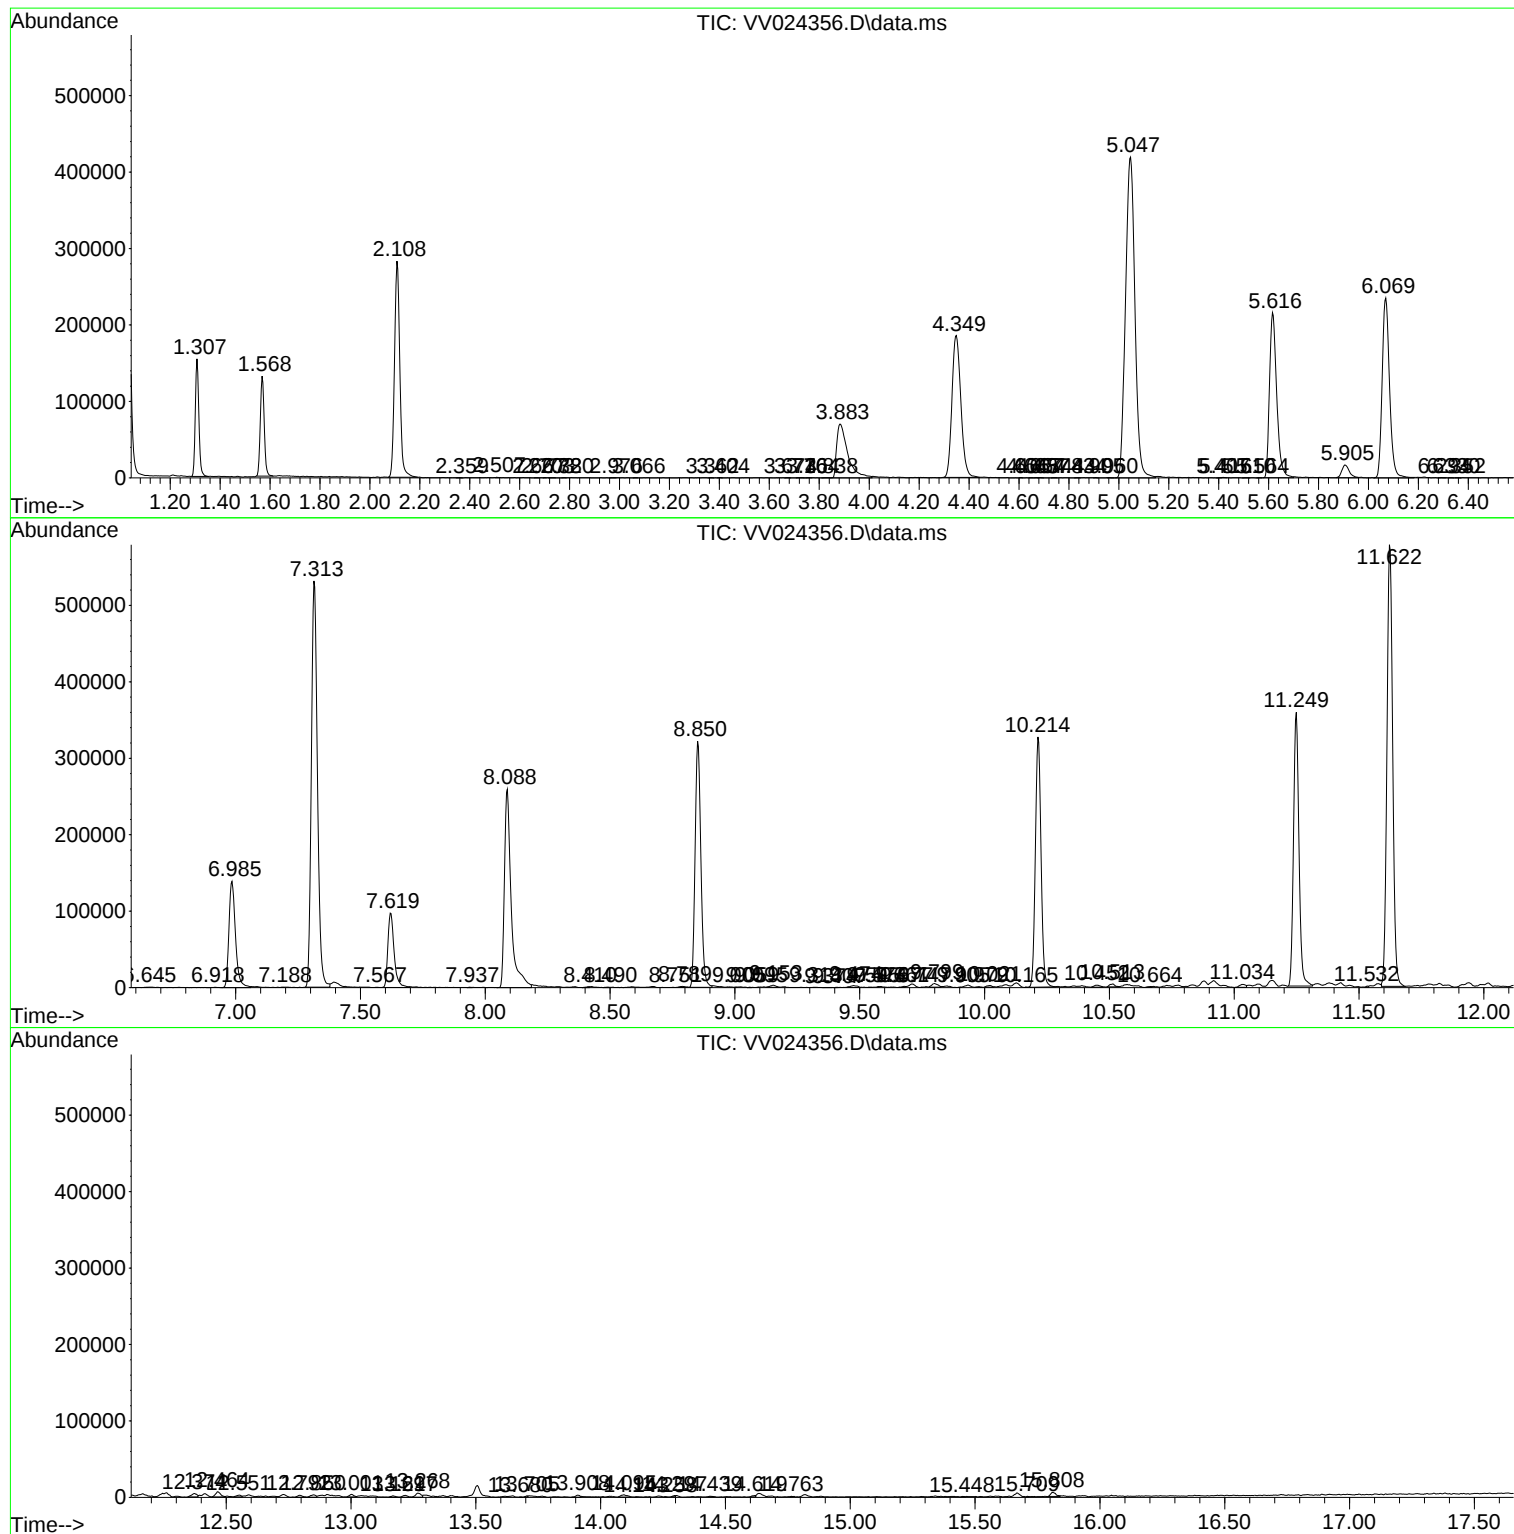

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024356.D
Acq On : 13 Jan 2022 17:57
Operator : SY/MD
Sample : N1115-16ME 10X
Misc : 6.56g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS6ME









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propanoic acid, 2,2,3-trich... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.905	4.04 ug/L	34865	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, 2,2,3-trichloro-...	190	C4H5Cl3O2	004749-35-3	50
2			Ethylene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	35
3			4-Chloro-3-fluoropyridine	131	C5H3ClFN	002546-56-7	32
4			Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	25
5			2-Chloro-4-fluoropyridine	131	C5H3ClFN	1000484-44-8	23

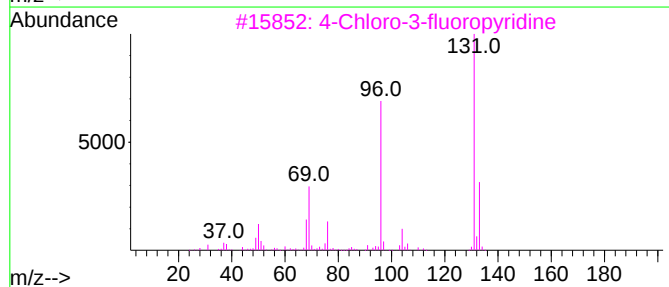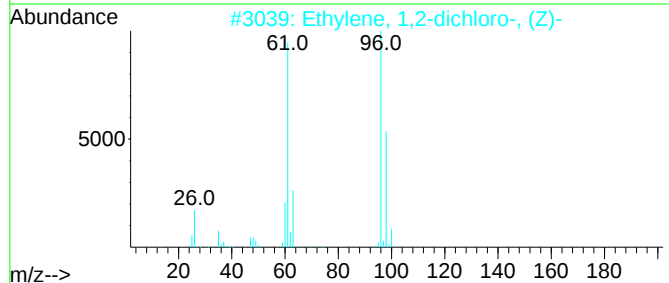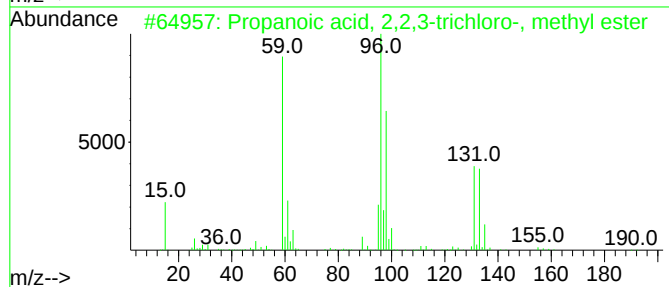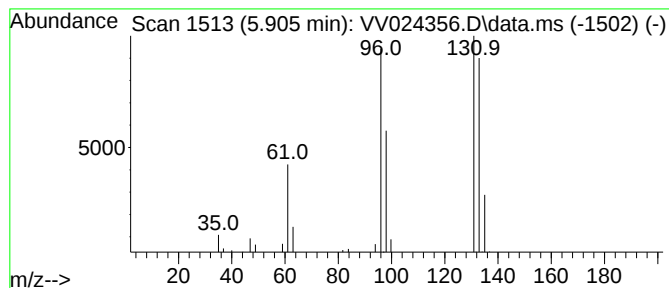

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
Data File : VV024356.D
Acq On : 13 Jan 2022 17:57
Operator : SY/MD
Sample : N1115-16ME 10X
Misc : 6.56g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propanoic acid,...	5.905	4.0	ug/L	34865	1	5.616	431644	50.0