
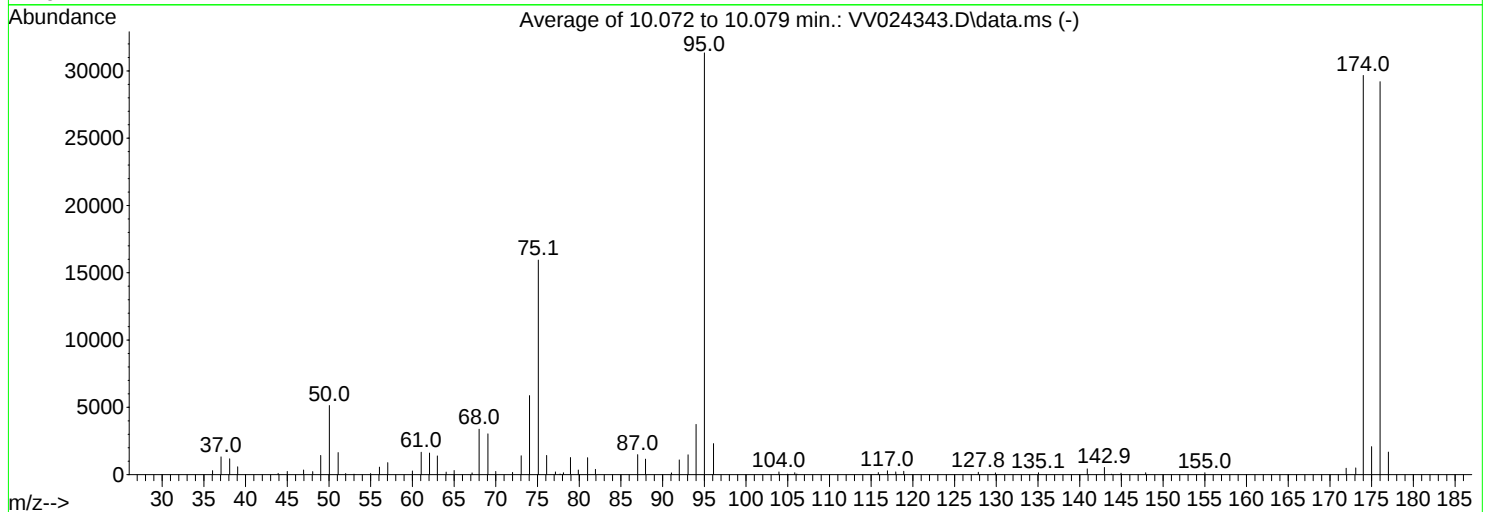


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011322\
 Data File : VV024343.D
 Acq On : 13 Jan 2022 10:10
 Operator : SY/MD
 Sample : BFB254
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB254

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis
 Last Update : Thu Jan 20 01:01:42 2022

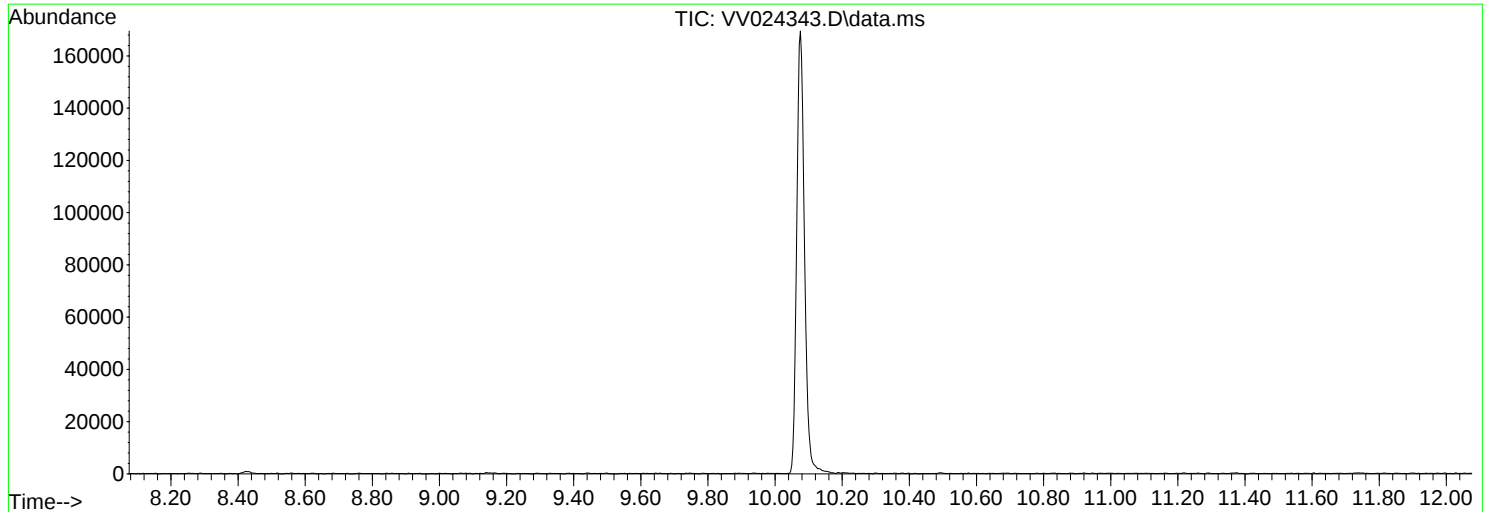

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	5132	PASS
75	95	30	80	50.9	15948	PASS
95	95	100	100	100.0	31341	PASS
96	95	5	9	7.4	2311	PASS
173	174	0.00	2	1.7	505	PASS
174	95	50	120	94.6	29661	PASS
175	174	5	9	7.0	2079	PASS
176	174	95	105	98.5	29205	PASS
177	176	5	10	5.7	1677	PASS

m/z	Abundance
44.00	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
36.10	260.0
37.00	1233.0
38.10	1206.0
39.10	598.0
43.90	309.0
45.00	245.0
46.90	368.0
48.10	224.0
49.00	1306.0
50.00	4752.0
51.10	1529.0
56.00	506.0
57.00	880.0
60.00	263.0
61.00	1528.0
62.10	1569.0
63.00	1336.0
64.10	160.0
65.00	297.0
67.10	150.0
68.00	3212.0
69.00	2867.0
70.00	223.0
72.00	202.0
73.10	1361.0
74.10	5509.0
75.10	15147.0
76.10	1273.0
77.10	184.0
78.10	175.0
78.90	1202.0
79.90	320.0
81.00	1244.0
82.00	370.0
87.00	1431.0
88.00	1188.0
91.00	131.0
92.00	1079.0
93.10	1463.0
94.00	3659.0
95.00	30264.0
96.10	2281.0
103.90	155.0
105.70	131.0
106.10	147.0
115.80	149.0
116.90	265.0
118.00	211.0
118.90	274.0
127.80	175.0
130.00	112.0
135.00	129.0
140.80	441.0
143.00	492.0
143.80	112.0
144.90	205.0
147.90	127.0
155.00	158.0
172.00	503.0
173.10	406.0
174.00	29416.0
175.00	2042.0
176.00	29024.0
177.00	1548.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
36.00	293.0
37.00	1359.0
38.10	1239.0
39.00	601.0
43.90	277.0
45.00	224.0
47.00	361.0
48.10	219.0
49.00	1502.0
50.00	5283.0
51.10	1698.0
52.00	124.0
55.00	109.0
56.10	590.0
57.10	950.0
60.00	278.0
61.10	1744.0
62.10	1667.0
63.00	1431.0
64.00	208.0
65.00	317.0
67.20	150.0
68.00	3519.0
69.00	3146.0
70.00	234.0
72.00	186.0
73.10	1435.0
74.10	6173.0
75.10	16400.0
76.10	1442.0
77.20	210.0
78.10	145.0
78.90	1314.0
79.90	347.0
81.00	1304.0
81.90	406.0
87.00	1553.0
88.00	1204.0
91.00	130.0
92.00	1128.0
93.00	1501.0
94.00	3811.0
95.00	32328.0
96.10	2418.0
104.00	205.0
105.90	148.0
115.80	168.0
117.00	300.0
117.90	223.0
118.90	258.0
127.80	195.0
129.90	115.0
135.10	146.0
140.90	425.0
142.90	533.0
145.00	134.0
147.90	136.0
155.00	161.0
172.00	494.0
173.10	521.0
174.00	30464.0
175.00	2134.0
176.00	30088.0
177.00	1723.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
36.00	336.0
37.10	1375.0
38.10	1099.0
39.00	543.0
43.90	241.0
45.00	252.0
47.00	313.0
48.00	248.0
49.00	1479.0
50.10	5362.0
51.10	1702.0
52.00	138.0
53.00	105.0
55.00	136.0
56.10	571.0
57.10	859.0
60.00	289.0
61.10	1724.0
62.00	1567.0
63.00	1416.0
64.00	222.0
65.00	323.0
67.20	112.0
68.00	3413.0
69.10	3074.0
70.00	264.0
72.00	128.0
73.00	1399.0
74.00	5925.0
75.10	16296.0
76.10	1551.0
77.10	207.0
77.70	126.0
78.10	127.0
79.00	1294.0
79.90	364.0
81.00	1246.0
81.90	390.0
87.00	1478.0
87.90	1086.0
91.10	117.0
92.00	1076.0
93.00	1480.0
94.00	3747.0
95.00	31432.0
96.10	2235.0
104.00	236.0
105.00	123.0
105.90	160.0
115.90	149.0
117.00	276.0
117.90	193.0
118.90	213.0
127.90	171.0
129.80	158.0
135.10	150.0
141.00	420.0
142.90	569.0
147.90	157.0
155.00	123.0
171.90	436.0
173.10	588.0
174.00	29104.0
175.00	2062.0
176.00	28504.0
177.00	1759.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254