

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011420\
 Data File : VV014297.D
 Acq On : 14 Jan 2020 15:57
 Operator : SY/MD
 Sample : L1101-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 1/15/2020 12:28:36 PM

Quant Time: Jan 14 22:23:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 14 22:19:33 2020
 Response via : Initial Calibration

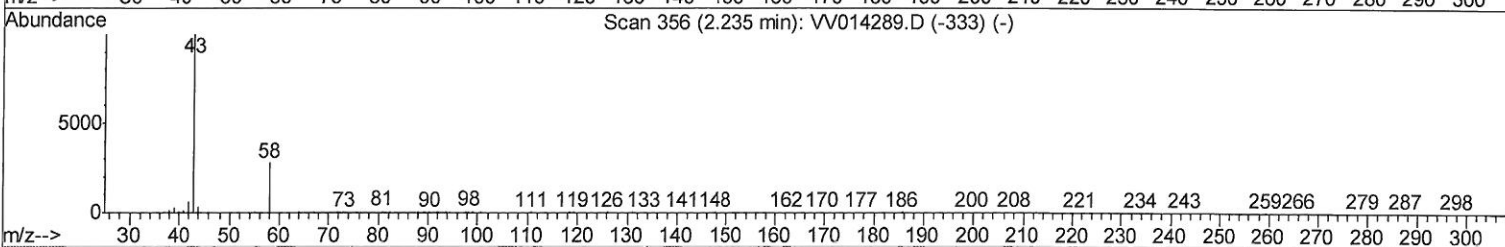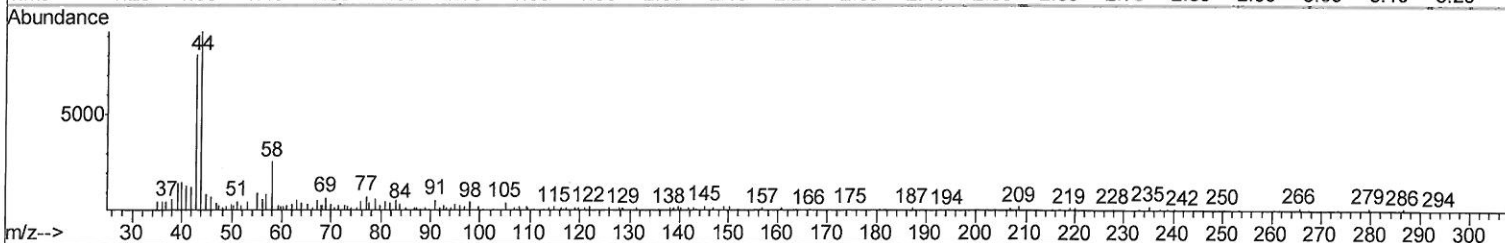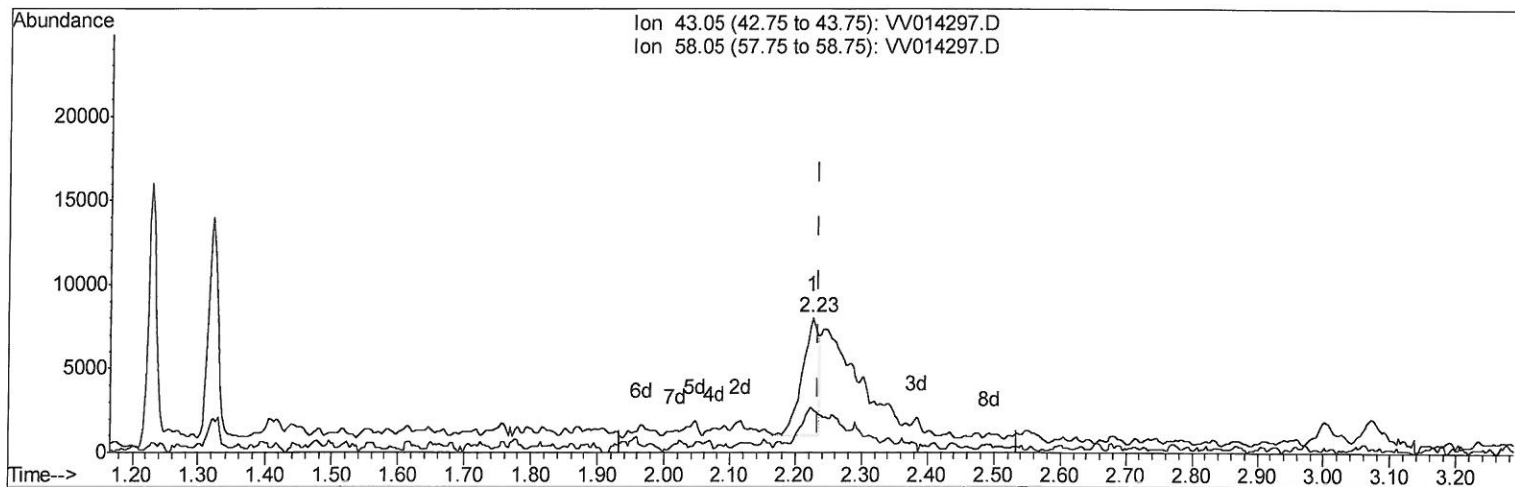

TIC: VV014297.D

(13) Acetone (T)

2.225min (-0.010) 1.16ug/L

response 11937

Ion	Exp%	Act%
43.05	100	100
58.05	33.00	39.95
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011420\
 Data File : VV014297.D
 Acq On : 14 Jan 2020 15:57
 Operator : SY/MD
 Sample : L1101-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 1/15/2020 12:28:36 PM

Quant Time: Jan 14 22:23:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 14 22:19:33 2020
 Response via : Initial Calibration

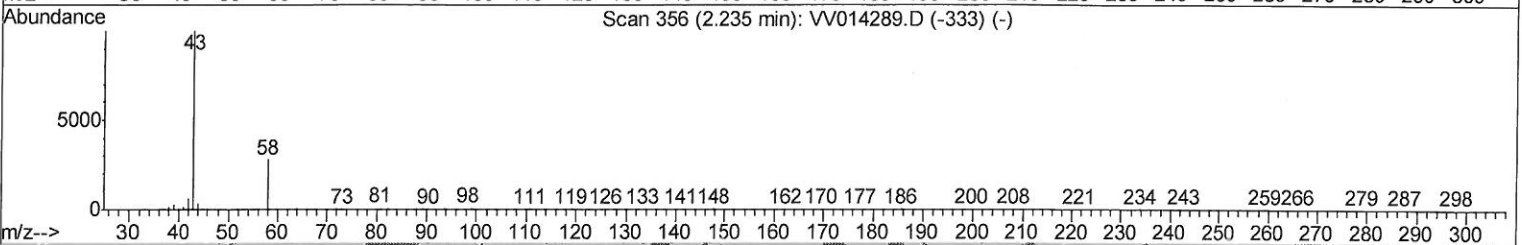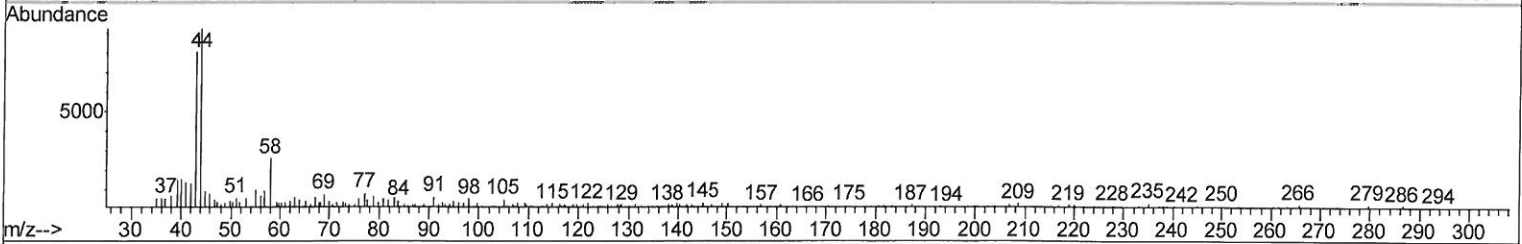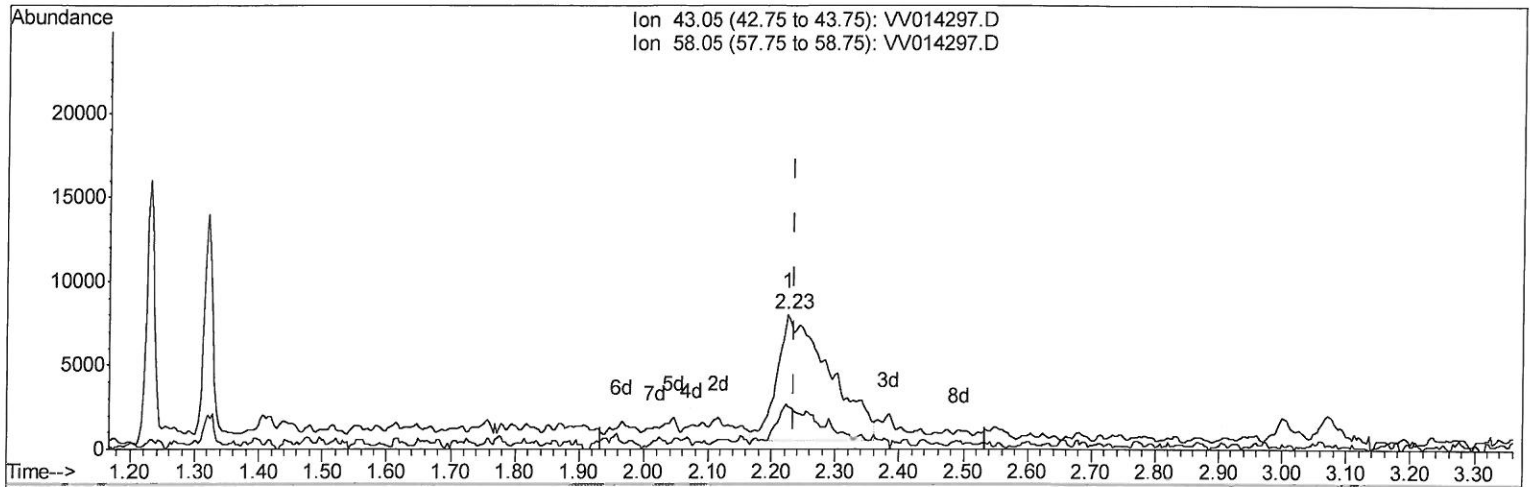

TIC: VV014297.D

(13) Acetone (T)

2.225min (-0.010) 4.25ug/L m

response 43571

Ion	Exp%	Act%
43.05	100	100
58.05	33.00	10.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011420\
 Data File : VV014297.D
 Acq On : 14 Jan 2020 15:57
 Operator : SY/MD
 Sample : L1101-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 1/15/2020 12:28:36 PM

Quant Time: Jan 14 23:08:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 14 22:19:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	885696	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	823233	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	367527	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	272209	4.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.80%
7) Chloroethane-d5	1.59	69	220711	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.20%
11) 1,1-Dichloroethene-d2	2.13	63	340777	3.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.60%
20) 2-Butanone-d5	3.96	46	745290	50.06	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.12%
24) Chloroform-d	4.40	84	584321	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.08	65	298202	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
32) Benzene-d6	5.10	84	1241404	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	6.11	67	389014	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	7.35	98	1104637	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
43) trans-1,3-Dichloropropene-	7.66	79	160157	4.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.00%
46) 2-Hexanone-d5	8.13	63	675379	47.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.68%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	256668	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	356934	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%

Target Compounds

				Ovalue	
3) Chloromethane	1.26	50	11053	0.167 ug/L	86
13) Acetone	2.23	43	43571m	4.250 ug/L	94
16) Methylene chloride	2.54	84	40434	0.628 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011420\
Data File : VV014297.D
Acq On : 14 Jan 2020 15:57
Operator : SY/MD
Sample : L1101-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
1/15/2020 12:28:36 PM

Quant Time: Jan 14 23:08:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 14 22:19:33 2020
Response via : Initial Calibration

