

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011420\
 Data File : VV014299.D
 Acq On : 14 Jan 2020 17:03
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Quant Time: Jan 14 23:16:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 14 22:19:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	1042398	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	945959	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	439037	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	246044	3.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.40%
7) Chloroethane-d5	1.58	69	196095	3.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.60%
11) 1,1-Dichloroethene-d2	2.13	63	296983	2.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.20%#
20) 2-Butanone-d5	3.96	46	657388	37.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.04%
24) Chloroform-d	4.40	84	533047	3.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.60%
26) 1,2-Dichloroethane-d4	5.08	65	265490	3.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.20%
32) Benzene-d6	5.09	84	1117896	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.20%
36) 1,2-Dichloropropane-d6	6.11	67	352280	4.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.60%
41) Toluene-d8	7.35	98	1012676	3.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.60%
43) trans-1,3-Dichloropropene-	7.66	79	145421	3.76	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.20%
46) 2-Hexanone-d5	8.13	63	618554	37.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.48%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	234838	3.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	76.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	326876	3.97	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.40%#


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	31883	0.421 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV011420\
Data File : VV014299.D
Acq On : 14 Jan 2020 17:03
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Time: Jan 14 23:16:52 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 14 22:19:33 2020
Response via : Initial Calibration

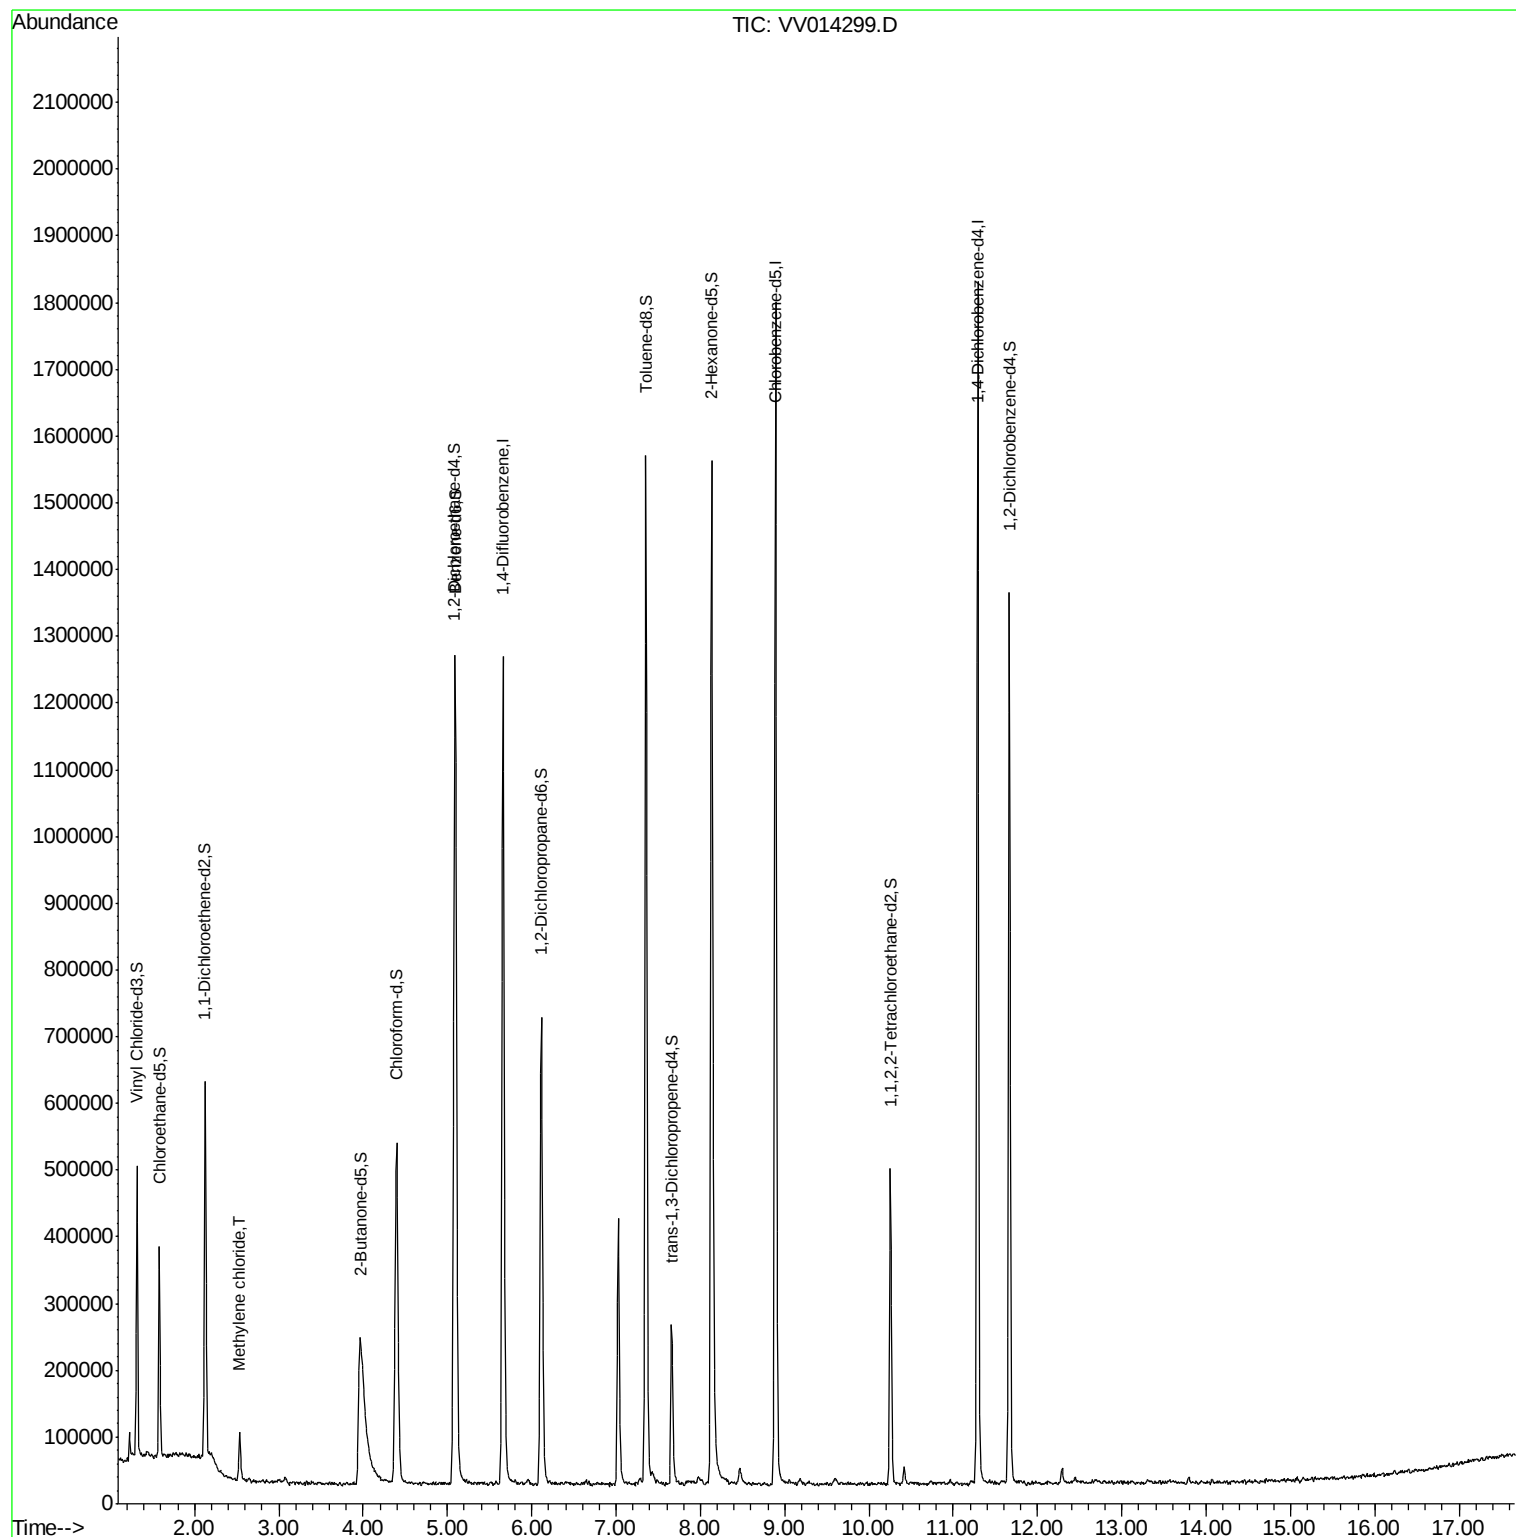

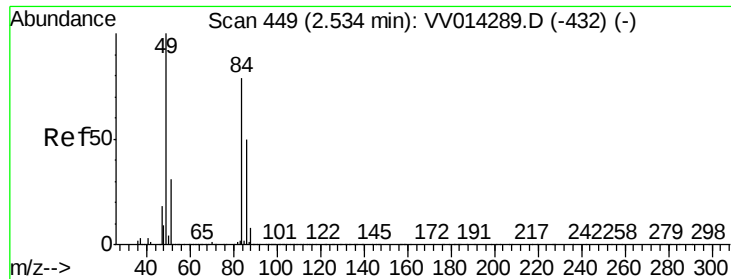

#16
 Methvlene chloride
 Concen: 0.421 ug/L
 RT: 2.53 min Scan# 449
 Delta R.T. 0.00 min
 Lab File: VV014299.D
 Acq: 14 Jan 2020 17:03

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Tot Ion: 84 Resp: 31883
 Ion Ratio Lower Upper
 84 100
 86 66.9 43.1 80.1
 49 124.3 82.1 152.5

