

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011420\
 Data File : VV014301.D
 Acq On : 14 Jan 2020 17:50
 Operator : SY/MD
 Sample : L1118-15
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jan 14 23:22:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 14 22:19:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	896551	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	814742	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	368458	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	245558	3.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.40%
7) Chloroethane-d5	1.58	69	202663	4.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.60%
11) 1,1-Dichloroethene-d2	2.13	63	306337	3.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.20%
20) 2-Butanone-d5	3.96	46	693578	46.03	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.06%
24) Chloroform-d	4.40	84	542267	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.08	65	269110	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
32) Benzene-d6	5.10	84	1143859	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.12	67	359276	4.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.40%
41) Toluene-d8	7.36	98	1012918	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
43) trans-1,3-Dichloropropene-	7.66	79	142449	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.13	63	634777	44.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.92%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	237151	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	322860	4.67	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.40%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	11586	0.178 ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV011420\
Data File : VV014301.D
Acq On : 14 Jan 2020 17:50
Operator : SY/MD
Sample : L1118-15
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jan 14 23:22:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 14 22:19:33 2020
Response via : Initial Calibration

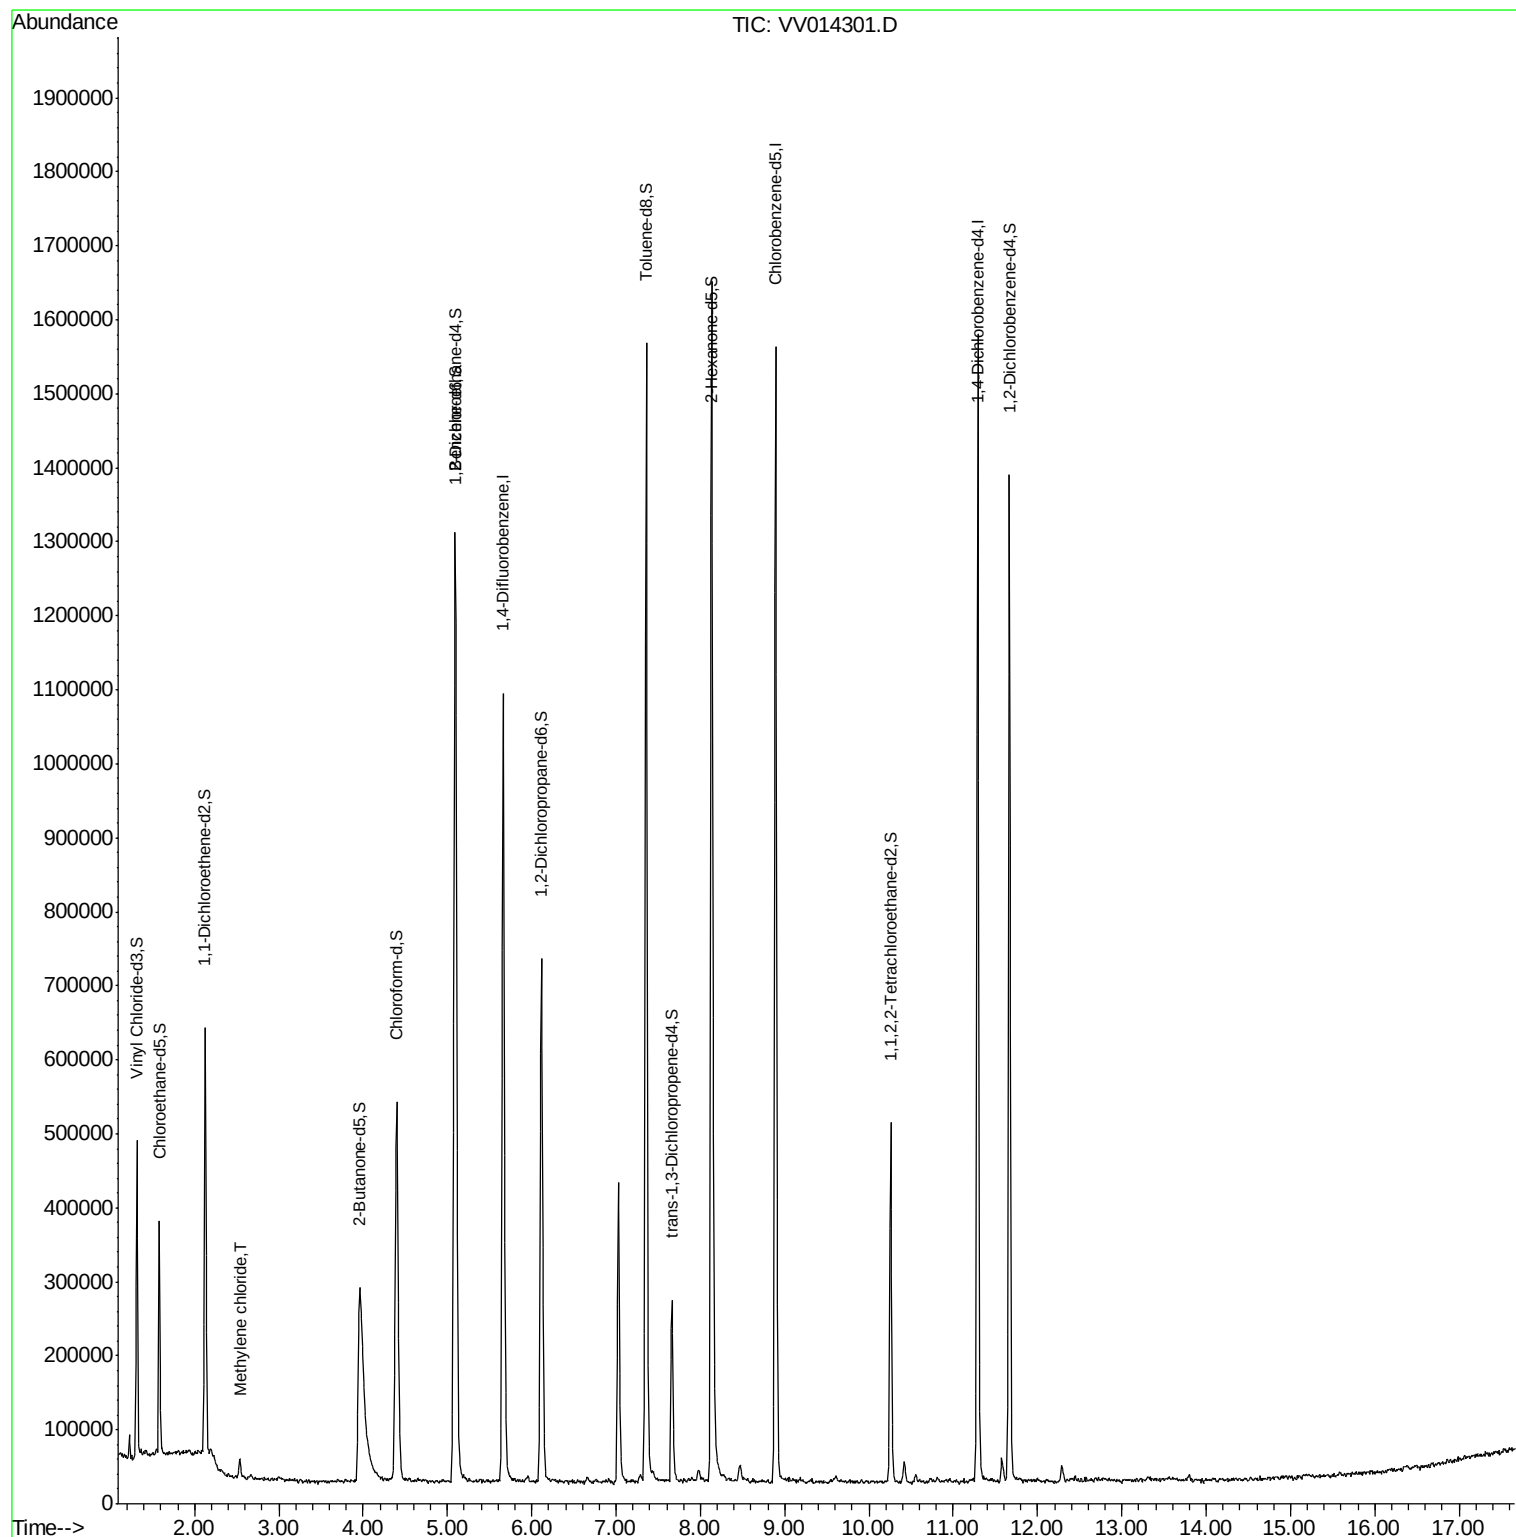

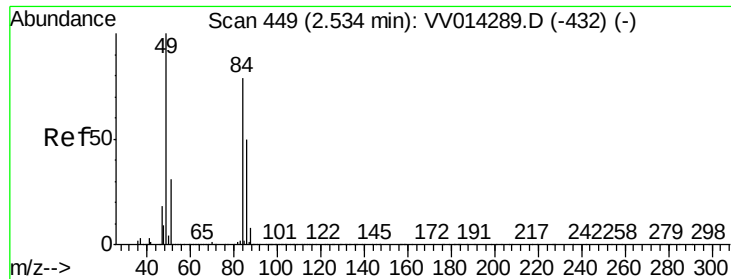

#16
 Methylene chloride
 Concen: 0.178 ug/L
 RT: 2.53 min Scan# 449
 Delta R.T. 0.00 min
 Lab File: VV014301.D
 Acq: 14 Jan 2020 17:50

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 11586
 Ion Ratio Lower Upper
 84 100
 86 63.1 43.1 80.1
 49 142.1 82.1 152.5

