

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011422\
 Data File : VV024361.D
 Acq On : 14 Jan 2022 15:10
 Operator : SY/MD
 Sample : VV0114WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK294

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M

Title : VOC Analysis

Signal : TIC: VV024361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	120158	118776	13.60%	1.684%
2	1.568	157	164	176	rVB	100824	112409	12.87%	1.594%
3	2.108	321	332	357	rVB	214823	322742	36.94%	4.575%
4	2.214	363	365	370	rVB2	429	213	0.02%	0.003%
5	2.291	386	389	390	rBV2	404	236	0.03%	0.003%
6	2.507	447	456	466	rVB2	3086	4477	0.51%	0.063%
7	2.690	510	513	515	rBV	268	201	0.02%	0.003%
8	2.706	515	518	526	rVB2	327	429	0.05%	0.006%
9	2.738	526	528	531	rBV	247	207	0.02%	0.003%
10	2.892	572	576	580	rBB	323	238	0.03%	0.003%
11	2.976	598	602	604	rBV	178	176	0.02%	0.002%
12	3.044	619	623	626	rBV	196	193	0.02%	0.003%
13	3.134	649	651	656	rBB	247	198	0.02%	0.003%
14	3.182	659	666	672	rBB2	316	494	0.06%	0.007%
15	3.236	676	683	686	rBV	169	263	0.03%	0.004%
16	3.275	691	695	698	rBV	166	172	0.02%	0.002%
17	3.545	777	779	782	rBV	239	156	0.02%	0.002%
18	3.696	821	826	827	rBV	323	215	0.02%	0.003%
19	3.796	852	857	859	rBV	131	163	0.02%	0.002%
20	3.880	872	883	916	rBV	58632	175037	20.04%	2.481%
21	4.066	939	941	942	rBV2	527	176	0.02%	0.002%
22	4.343	1012	1027	1059	rBV2	151113	364564	41.73%	5.168%
23	4.600	1105	1107	1111	rVB2	395	206	0.02%	0.003%
24	4.661	1123	1126	1129	rVB3	288	200	0.02%	0.003%
25	4.703	1135	1139	1141	rBV3	333	248	0.03%	0.004%
26	4.738	1146	1150	1153	rBB	254	176	0.02%	0.002%
27	4.825	1174	1177	1180	rBV	314	288	0.03%	0.004%
28	4.870	1188	1191	1195	rBV2	184	169	0.02%	0.002%
29	5.040	1227	1244	1272	rBV2	336136	873591	100.00%	12.384%
30	5.220	1298	1300	1304	rBV2	371	279	0.03%	0.004%
31	5.297	1321	1324	1328	rVB2	304	176	0.02%	0.002%
32	5.362	1339	1344	1349	rVB2	438	538	0.06%	0.008%
33	5.404	1355	1357	1359	rBV	379	213	0.02%	0.003%
34	5.471	1371	1378	1380	rBV2	270	299	0.03%	0.004%
35	5.613	1409	1422	1443	rBV	303671	611856	70.04%	8.674%
36	5.902	1502	1512	1528	rVV2	14821	30499	3.49%	0.432%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011422\
 Data File : VV024361.D
 Acq On : 14 Jan 2022 15:10
 Operator : SY/MD
 Sample : VV0114WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK294

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	6.008	1541	1545	1548	rBB2	290	273	0.03%	0.004%
38	6.063	1549	1562	1590	rBV	188678	390995	44.76%	5.543%
39	6.201	1603	1605	1613	rVB4	767	875	0.10%	0.012%
40	6.268	1623	1626	1629	rVB2	198	157	0.02%	0.002%
41	6.378	1657	1660	1664	rVB2	311	215	0.02%	0.003%
42	6.407	1665	1669	1670	rBV	248	183	0.02%	0.003%
43	6.455	1680	1684	1687	rBB	279	206	0.02%	0.003%
44	6.555	1713	1715	1722	rBV	191	268	0.03%	0.004%
45	6.616	1731	1734	1737	rBV2	271	214	0.02%	0.003%
46	6.635	1737	1740	1744	rVV2	514	434	0.05%	0.006%
47	6.725	1763	1768	1769	rBV	450	231	0.03%	0.003%
48	6.748	1772	1775	1778	rVV	251	165	0.02%	0.002%
49	6.828	1796	1800	1803	rBV2	280	269	0.03%	0.004%
50	6.982	1837	1848	1869	rBV	110830	202369	23.17%	2.869%
51	7.143	1895	1898	1901	rVB	272	191	0.02%	0.003%
52	7.194	1909	1914	1915	rBV2	708	487	0.06%	0.007%
53	7.236	1925	1927	1931	rVB	375	240	0.03%	0.003%
54	7.310	1937	1950	1970	rBV	411061	723904	82.87%	10.262%
55	7.619	2035	2046	2069	rBV	77893	138012	15.80%	1.957%
56	7.751	2084	2087	2089	rBV2	559	365	0.04%	0.005%
57	7.850	2116	2118	2120	rBV2	241	157	0.02%	0.002%
58	8.024	2170	2172	2175	rBV	322	159	0.02%	0.002%
59	8.085	2181	2191	2206	rBV	200068	363751	41.64%	5.157%
60	8.349	2268	2273	2275	rBV	507	407	0.05%	0.006%
61	8.407	2288	2291	2293	rBV2	460	247	0.03%	0.004%
62	8.506	2318	2322	2325	rBV	286	290	0.03%	0.004%
63	8.686	2376	2378	2384	rVV	227	190	0.02%	0.003%
64	8.712	2384	2386	2392	rVB	285	203	0.02%	0.003%
65	8.776	2402	2406	2409	rVB	252	202	0.02%	0.003%
66	8.850	2417	2429	2459	rBV	457793	741797	84.91%	10.516%
67	9.018	2477	2481	2483	rBV2	482	305	0.03%	0.004%
68	9.201	2535	2538	2541	rVB	258	188	0.02%	0.003%
69	9.223	2542	2545	2547	rBV	331	229	0.03%	0.003%
70	9.252	2551	2554	2557	rBV2	221	189	0.02%	0.003%
71	9.416	2602	2605	2607	rBV	194	157	0.02%	0.002%
72	9.580	2652	2656	2659	rBV	307	226	0.03%	0.003%
73	9.673	2681	2685	2689	rBV	194	206	0.02%	0.003%
74	9.892	2749	2753	2758	rBV2	242	170	0.02%	0.002%
75	9.934	2763	2766	2770	rBV2	359	236	0.03%	0.003%
76	10.127	2817	2826	2836	rBV4	2010	2991	0.34%	0.042%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011422\
 Data File : VV024361.D
 Acq On : 14 Jan 2022 15:10
 Operator : SY/MD
 Sample : VV0114WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK294

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	10.214	2841	2853	2870	rBV	261769	407892	46.69%	5.782%
78	10.368	2897	2901	2905	rBV	242	247	0.03%	0.004%
79	10.445	2921	2925	2927	rBV	327	183	0.02%	0.003%
80	10.580	2962	2967	2968	rBV3	493	375	0.04%	0.005%
81	10.735	3011	3015	3017	rBV	243	183	0.02%	0.003%
82	10.918	3063	3072	3078	rBV6	1449	2183	0.25%	0.031%
83	11.117	3132	3134	3137	rBV2	254	179	0.02%	0.003%
84	11.140	3138	3141	3142	rBV	553	328	0.04%	0.005%
85	11.181	3151	3154	3155	rBV2	332	202	0.02%	0.003%
86	11.249	3163	3175	3191	rBV	476231	731312	83.71%	10.367%
87	11.571	3272	3275	3278	rVB2	304	184	0.02%	0.003%
88	11.622	3278	3291	3307	rBV	456363	714318	81.77%	10.127%
89	11.718	3318	3321	3328	rVB3	497	401	0.05%	0.006%
90	11.776	3336	3339	3341	rBV2	329	237	0.03%	0.003%
91	12.378	3523	3526	3529	rBV	196	158	0.02%	0.002%
92	12.564	3581	3584	3588	rBV	307	191	0.02%	0.003%
93	12.654	3610	3612	3616	rVB	335	213	0.02%	0.003%
94	13.268	3798	3803	3810	rVB4	706	884	0.10%	0.013%
95	13.329	3819	3822	3828	rVB	243	167	0.02%	0.002%
96	13.426	3851	3852	3858	rVB2	336	175	0.02%	0.002%
97	13.464	3861	3864	3867	rBV2	217	186	0.02%	0.003%
98	13.609	3906	3909	3912	rBV2	301	200	0.02%	0.003%
99	14.651	4229	4233	4235	rBV2	320	306	0.04%	0.004%
100	15.226	4409	4412	4417	rBV2	504	405	0.05%	0.006%


Sum of corrected areas: 7053935

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011422\
Data File : VV024361.D
Acq On : 14 Jan 2022 15:10
Operator : SY/MD
Sample : VV0114WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

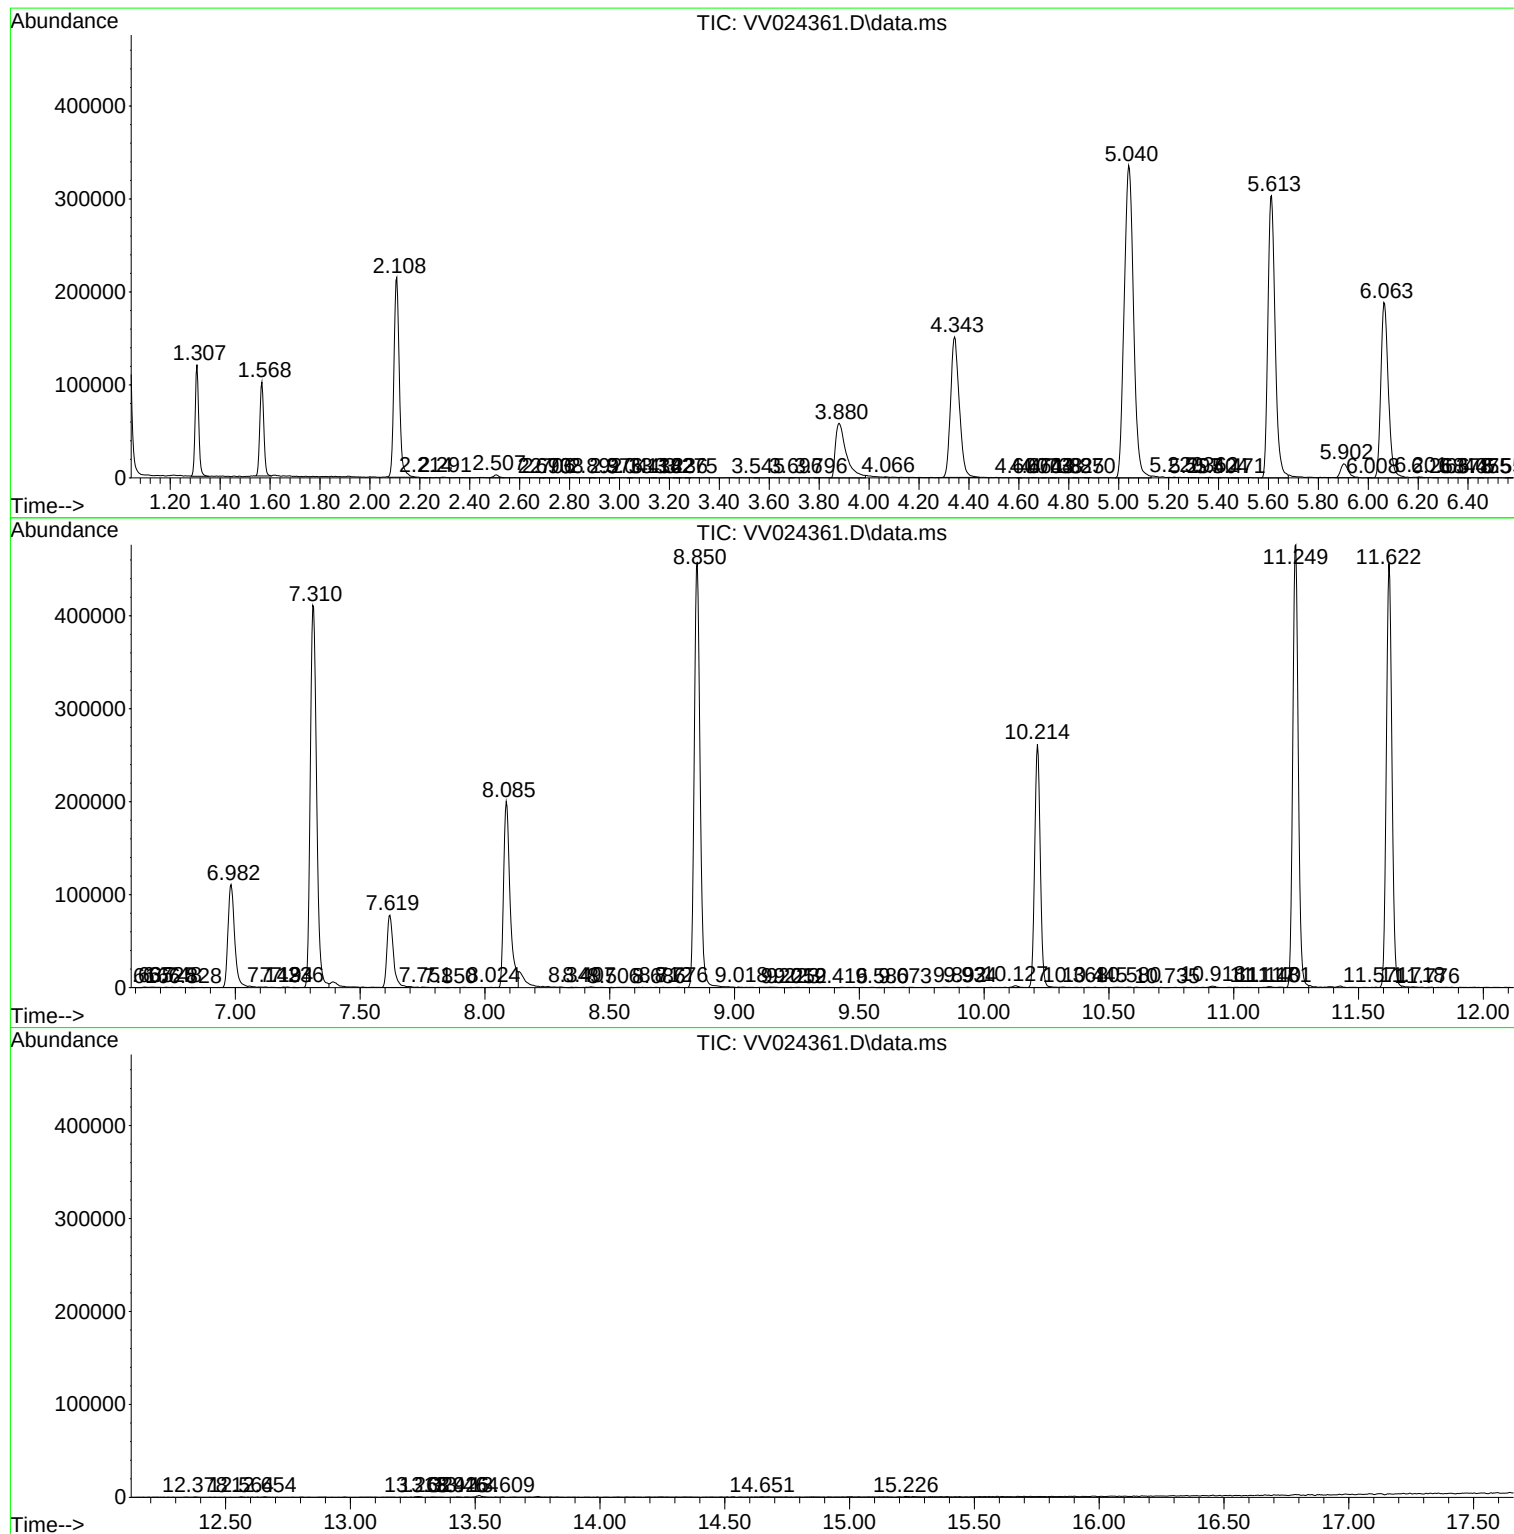

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011422\
Data File : VV024361.D
Acq On : 14 Jan 2022 15:10
Operator : SY/MD
Sample : VV0114WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011422\
Data File : VV024361.D
Acq On : 14 Jan 2022 15:10
Operator : SY/MD
Sample : VV0114WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------