
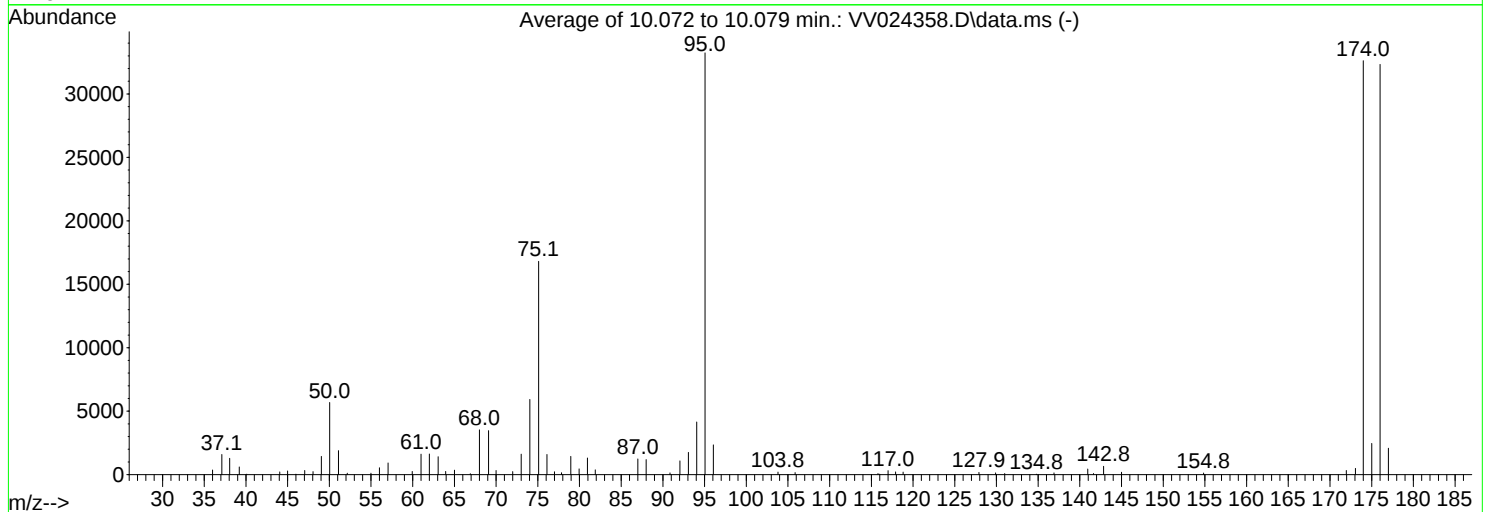


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011422\
 Data File : VV024358.D
 Acq On : 14 Jan 2022 09:31
 Operator : SY/MD
 Sample : BFB255
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB255

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis
 Last Update : Thu Jan 13 02:28:22 2022

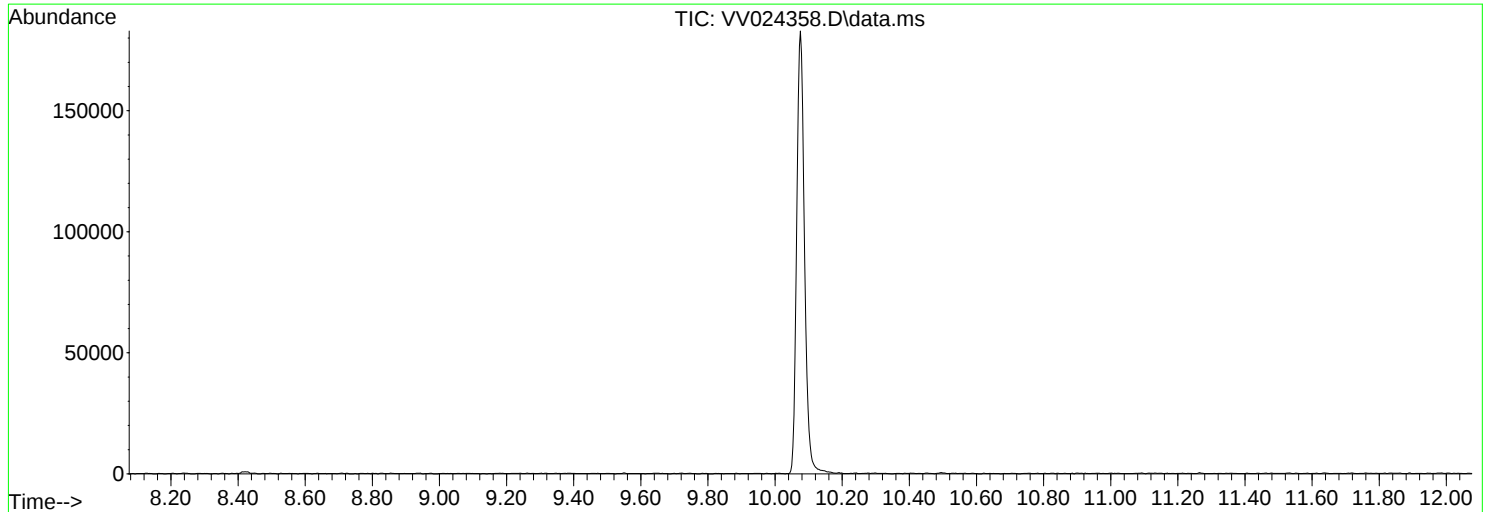

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	5692	PASS
75	95	30	80	50.6	16811	PASS
95	95	100	100	100.0	33237	PASS
96	95	5	9	7.1	2351	PASS
173	174	0.00	2	1.5	488	PASS
174	95	50	120	98.1	32613	PASS
175	174	5	9	7.5	2461	PASS
176	174	95	105	99.1	32323	PASS
177	176	5	10	6.4	2076	PASS

m/z	Abundance
44.10	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
36.00	350.0
37.10	1642.0
38.00	1338.0
39.20	607.0
44.00	417.0
45.00	251.0
47.10	327.0
48.00	231.0
49.10	1374.0
50.10	5953.0
51.10	1863.0
52.20	110.0
54.90	122.0
56.00	459.0
57.10	929.0
60.00	273.0
61.00	1610.0
62.00	1572.0
63.10	1450.0
63.90	246.0
65.00	327.0
66.90	109.0
68.00	3603.0
69.10	3446.0
70.00	294.0
72.10	236.0
73.00	1527.0
74.00	5972.0
75.10	16712.0
76.10	1677.0
77.00	266.0
77.90	155.0
79.00	1439.0
80.00	413.0
81.00	1268.0
81.90	376.0
87.00	1095.0
88.00	1169.0
90.90	144.0
92.10	1064.0
93.10	1693.0
94.00	4195.0
95.10	33416.0
96.10	2347.0
103.80	240.0
105.90	167.0
115.80	142.0
117.00	302.0
117.90	208.0
118.80	213.0
127.90	178.0
129.90	170.0
134.80	105.0
136.90	119.0
140.90	421.0
142.80	742.0
145.00	205.0
154.80	116.0
171.90	293.0
173.00	480.0
174.00	32144.0
175.00	2551.0
176.00	31688.0
177.00	2113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
36.00	381.0
37.10	1653.0
38.10	1329.0
39.20	632.0
44.00	369.0
45.00	301.0
46.00	101.0
47.10	330.0
48.10	249.0
49.00	1502.0
50.00	5813.0
51.10	1943.0
52.10	118.0
55.00	115.0
56.00	550.0
57.00	943.0
59.90	254.0
61.00	1668.0
62.00	1687.0
63.10	1453.0
63.90	276.0
65.00	348.0
66.90	129.0
68.00	3662.0
69.10	3552.0
70.00	359.0
71.90	231.0
73.00	1652.0
74.10	6096.0
75.10	17280.0
76.10	1647.0
77.00	242.0
77.90	151.0
79.00	1491.0
79.90	478.0
80.90	1323.0
81.90	398.0
87.00	1240.0
88.00	1175.0
90.90	147.0
92.00	1141.0
93.10	1806.0
94.10	4263.0
95.00	34200.0
96.10	2451.0
103.80	202.0
105.90	171.0
115.80	130.0
117.00	313.0
117.90	219.0
118.80	202.0
127.90	193.0
129.90	151.0
131.00	133.0
136.90	164.0
141.00	440.0
141.60	146.0
142.90	671.0
145.00	177.0
154.80	123.0
171.90	332.0
173.00	494.0
174.00	33648.0
175.00	2548.0
176.00	33184.0
177.00	2146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
36.00	355.0
37.10	1472.0
38.10	1210.0
39.20	571.0
40.10	109.0
44.10	274.0
45.00	338.0
47.00	319.0
48.10	255.0
49.00	1453.0
50.00	5310.0
51.10	1855.0
52.10	114.0
55.10	110.0
56.00	621.0
57.00	885.0
59.90	222.0
61.00	1545.0
62.00	1611.0
63.00	1329.0
64.00	247.0
65.00	368.0
68.00	3341.0
69.10	3388.0
70.00	334.0
72.00	245.0
73.00	1651.0
74.10	5725.0
75.10	16440.0
76.10	1457.0
77.00	177.0
77.80	136.0
78.90	1387.0
79.90	478.0
80.90	1360.0
81.90	378.0
87.00	1385.0
88.00	1198.0
90.80	145.0
92.00	1057.0
93.00	1769.0
94.10	4001.0
95.00	32096.0
96.00	2254.0
103.80	150.0
105.80	175.0
116.00	109.0
117.00	338.0
117.90	210.0
118.80	177.0
127.90	171.0
129.80	107.0
131.00	126.0
136.90	138.0
140.90	460.0
141.70	140.0
142.80	573.0
145.00	181.0
154.90	126.0
172.00	375.0
173.10	490.0
174.00	32048.0
175.00	2283.0
176.00	32096.0
177.00	1968.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255