

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011722\
 Data File : VW024374.D
 Acq On : 17 Jan 2022 13:11
 Operator : SY/MD
 Sample : N1168-12RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLX7RE

Quant Time: Jan 17 14:54:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	392253	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	366413	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	181628	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	90630	32.104	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	64.200%
7) Chloroethane-d5	1.568	69	67494	31.473	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	62.940%#
11) 1,1-Dichloroethene-d2	2.108	63	131295	24.885	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	49.780%#
21) 2-Butanone-d5	3.879	46	109506	69.624	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	69.620%
24) Chloroform-d	4.342	84	176880	34.283	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.560%#
26) 1,2-Dichloroethane-d4	5.027	65	116238	33.649	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	67.300%#
32) Benzene-d6	5.047	84	355721	37.202	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.400%
36) 1,2-Dichloropropane-d6	6.066	67	106086	39.588	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	79.180%
41) Toluene-d8	7.310	98	332676	35.934	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	71.860%#
43) trans-1,3-Dichloroprop...	7.616	79	53518	34.683	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.360%
47) 2-Hexanone-d5	8.085	63	72194	62.010	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	62.010%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	127918	33.403	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	66.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	138056	38.134	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.260%#
Target Compounds						
13) Acetone	2.175	43	6637	4.274	ug/L	Qvalue 48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
Data File : VV024374.D
Acq On : 17 Jan 2022 13:11
Operator : SY/MD
Sample : N1168-12RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLX7RE

Quant Time: Jan 17 14:54:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

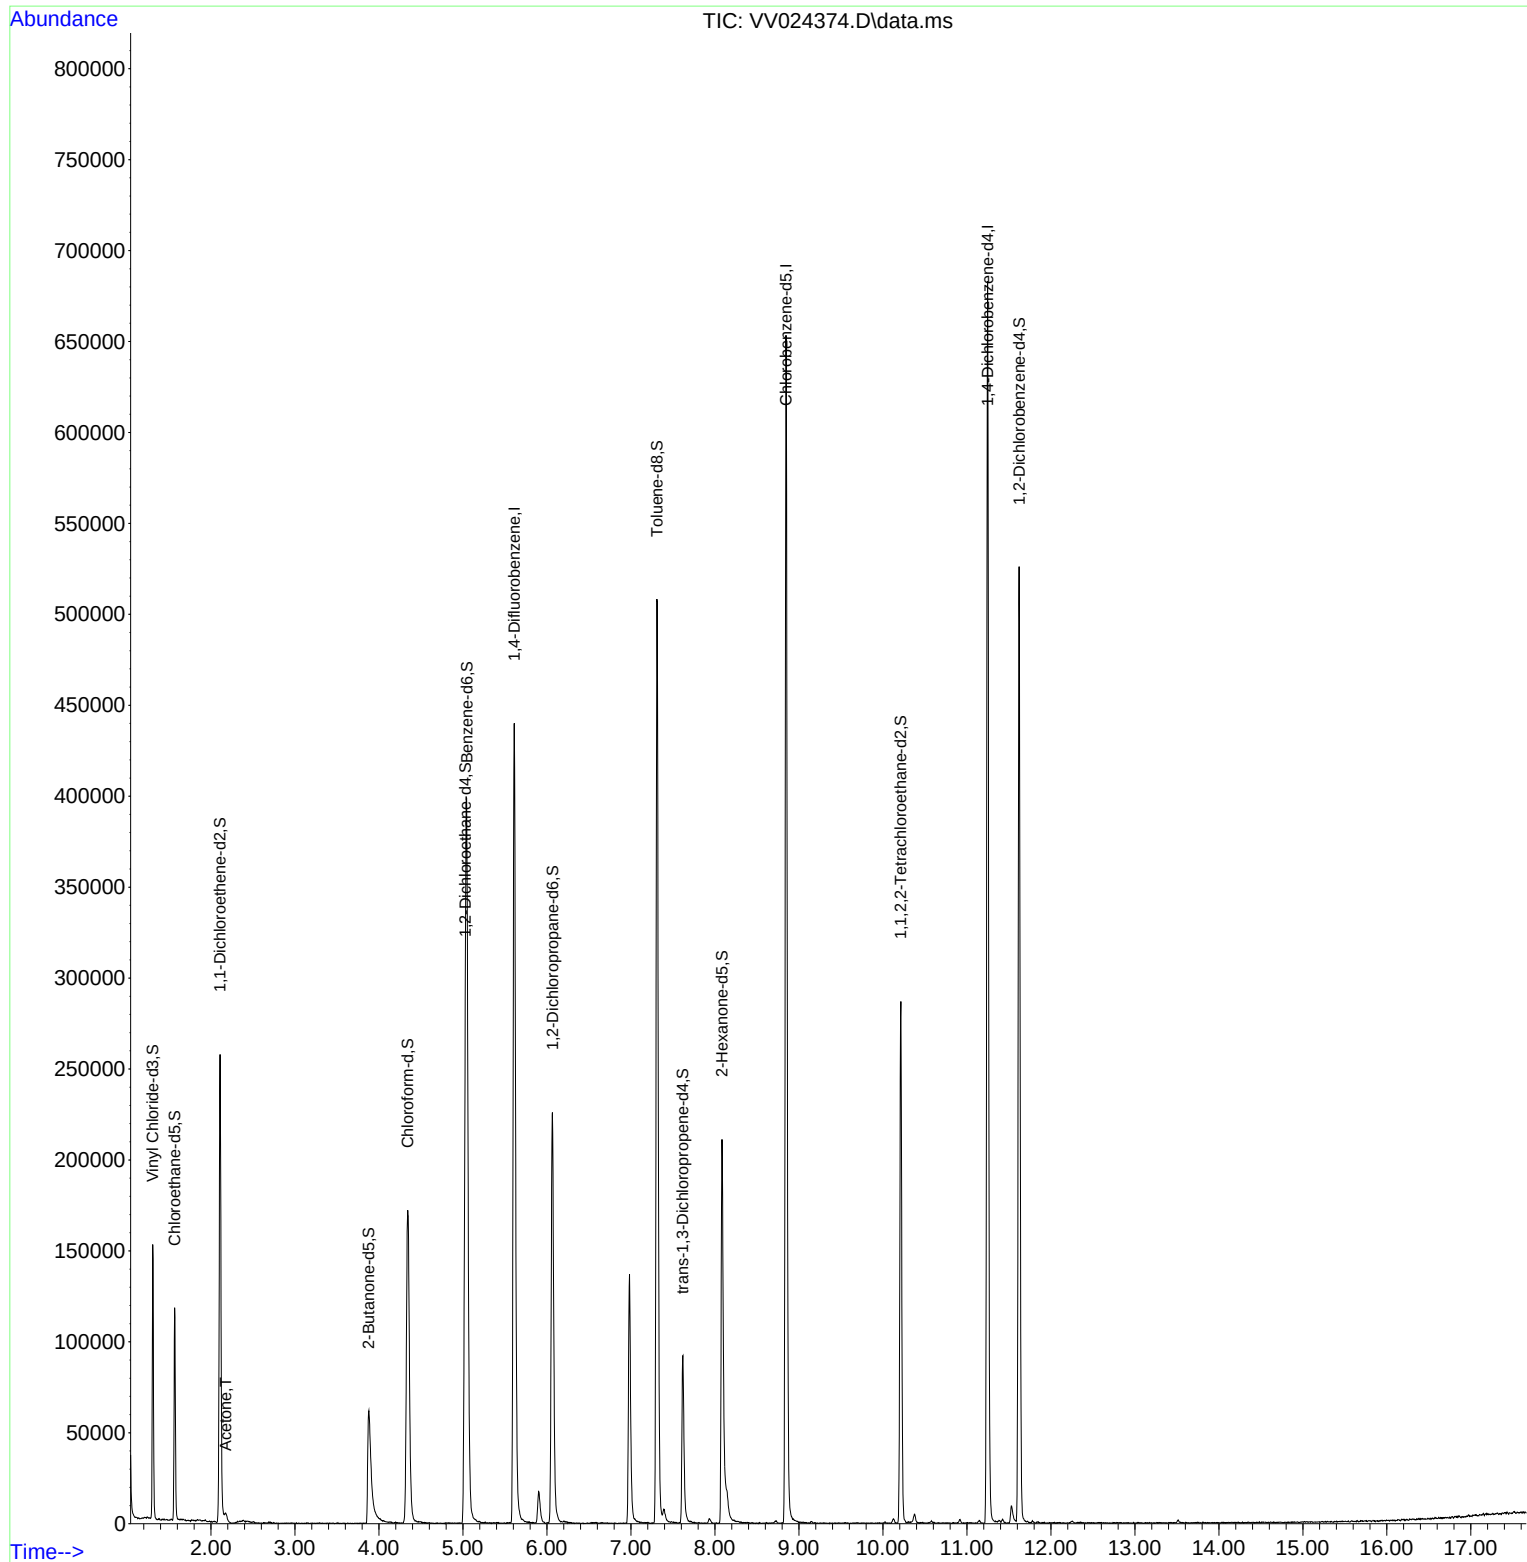

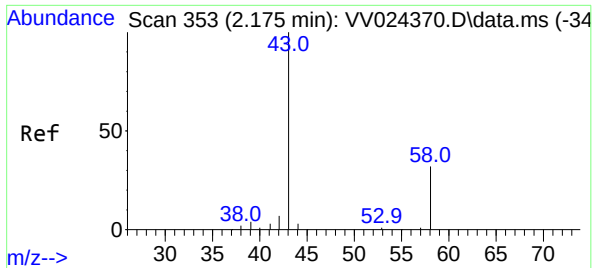

#13
Acetone
Concen: 4.274 ug/L
RT: 2.175 min Scan# 31
Delta R.T. -0.007 min
Lab File: VV024374.D
Acq: 17 Jan 2022 13:11

Instrument :
MSVOA_V
ClientSampleId :
BGLX7RE

Tgt Ion: 43 Resp: 6637
Ion Ratio Lower Upper
43 100
58 2.7 0.0 63.0

